


**Plug-in Type
Digital Indicating pH Meter
WIL-102-PH
Instruction Manual**

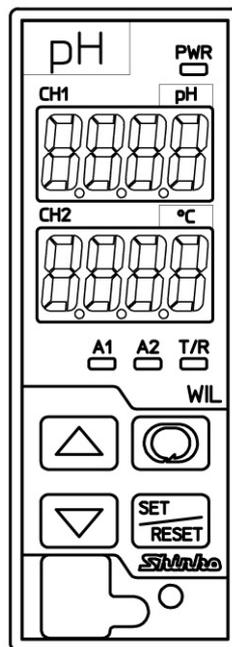

Shinko

Preface

Thank you for purchasing our WIL-102-PH, Plug-in Type Digital Indicating pH Meter.

This manual contains instructions for the mounting, functions, operations and notes when operating the WIL-102-PH. To ensure safe and correct use, thoroughly read and understand this manual before using this instrument.

To prevent accidents arising from the misuse of this instrument, please ensure the operator receives this manual.

Characters Used in This Manual

| | | | | | | | | | | | | | |
|---------------|----------|----------|----------|----------|----------|----------|----------|----------|----------|----------|----------|-----------|-----------|
| Indication | <i>1</i> | <i>0</i> | <i>1</i> | <i>2</i> | <i>3</i> | <i>4</i> | <i>5</i> | <i>6</i> | <i>7</i> | <i>8</i> | <i>9</i> | <i>°C</i> | <i>°F</i> |
| Number, °C/°F | -1 | 0 | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | °C | °F |
| Indication | <i>A</i> | <i>b</i> | <i>c</i> | <i>d</i> | <i>E</i> | <i>F</i> | <i>G</i> | <i>H</i> | <i>I</i> | <i>J</i> | <i>k</i> | <i>L</i> | <i>m</i> |
| Alphabet | A | B | C | D | E | F | G | H | I | J | K | L | M |
| Indication | <i>n</i> | <i>o</i> | <i>P</i> | <i>q</i> | <i>r</i> | <i>s</i> | <i>T</i> | <i>U</i> | <i>v</i> | <i>w</i> | <i>x</i> | <i>Y</i> | <i>Z</i> |
| Alphabet | N | O | P | Q | R | S | T | U | V | W | X | Y | Z |

Caution

- This instrument should be used in accordance with the specifications described in the manual. If it is not used according to the specifications, it may malfunction or cause a fire.
- Be sure to follow all of the warnings, cautions and notices. If they are not observed, serious injury or malfunction may occur.
- The contents of this instruction manual are subject to change without notice.
- Care has been taken to ensure that the contents of this instruction manual are correct, but if there are any doubts, mistakes or questions, please inform our sales department.
- This instrument is designed to be installed on a DIN rail within a control panel. If it is not, measures must be taken to ensure that the operator cannot touch power terminals or other high voltage sections.
- Any unauthorized transfer or copying of this document, in part or in whole, is prohibited.
- Shinko Technos Co., Ltd. is not liable for any damage or secondary damage(s) incurred as a result of using this product, including any indirect damage.

Safety Precautions (Be sure to read these precautions before using our products.)

The safety precautions are classified into 2 categories: “Warning” and “Caution”.

Depending on the circumstances, procedures indicated by  Caution may result in serious consequences, so be sure to follow the directions for usage.

Warning

Procedures which may lead to dangerous conditions and cause death or serious injury, if not carried out properly.

Caution

Procedures which may lead to dangerous conditions and cause superficial to medium injury or physical damage or may degrade or damage the product, if not carried out properly.



Warning

- To prevent an electrical shock or fire, only Shinko or other qualified service personnel may handle the inner assembly.
- To prevent an electrical shock, fire or damage to the instrument, parts replacement may only be undertaken by Shinko or other qualified service personnel.



SAFETY PRECAUTIONS

- To ensure safe and correct use, thoroughly read and understand this manual before using this instrument.
- This instrument is intended to be used for measuring equipment. Verify correct usage after purpose-of-use consultation with our agency or main office. (Never use this instrument for medical purposes with which human lives are involved.)
- External protection devices such as protective equipment against excessive temperature rise, etc. must be installed, as malfunction of this product could result in serious damage to the system or injury to personnel. Proper periodic maintenance is also required.
- This instrument must be used under the conditions and environment described in this manual. Shinko Technos Co., Ltd. does not accept liability for any injury, loss of life or damage occurring due to the instrument being used under conditions not otherwise stated in this manual.



Caution with Respect to Export Trade Control Ordinance

To avoid this instrument from being used as a component in, or as being utilized in the manufacture of weapons of mass destruction (i.e. military applications, military equipment, etc.), please investigate the end users and the final use of this instrument. In the case of resale, ensure that this instrument is not illegally exported.

PRECAUTIONS

1. Installation Precautions



Caution

This instrument is intended to be used under the following environmental conditions (IEC61010-1):

- Overvoltage category II, Pollution degree 2

Ensure the mounting location corresponds to the following conditions:

- A minimum of dust, and an absence of corrosive gases
- No flammable, explosive gases
- No mechanical vibrations or shocks
- No exposure to direct sunlight, an ambient temperature of 0 to 50°C (32 to 122°F) that does not change rapidly, and no icing
- An ambient non-condensing humidity of 35 to 85 %RH
- No large capacity electromagnetic switches or cables through which a large current is flowing.
- No water, oil, chemicals or the vapors of these substances can come into direct contact with the unit.
- If the WIL-102-PH is installed within a control panel, the ambient temperature of the unit – not the ambient temperature of the control panel – must be kept under 50°C. Otherwise the life of electronic parts (especially electrolytic capacitors) of the unit will be shortened.

Note: Do not install this instrument on or near flammable material even though the case of this instrument is made of flame-resistant resin.

2. Wiring Precautions



Caution

- Do not leave wire remnants in the instrument, as they could cause a fire or a malfunction.
- Use a solderless terminal with an insulation sleeve in which the M3 screw fits when wiring the WIL-102-PH.
- Tighten the terminal screw using the specified torque. If excessive force is applied to the screw when tightening, the terminal screw may be damaged.
- This instrument does not have a built-in power switch, circuit breaker and fuse.
It is necessary to install a power switch, circuit breaker and fuse near the instrument.
(Recommended fuse: Time-lag fuse, rated voltage 250 V AC, rated current 2 A)
- For a 24 V AC/DC power source, do not confuse polarity when using direct current (DC).
- Do not apply a commercial power source to the sensor which is connected to the input terminal nor allow the power source to come into contact with the sensor.
- Use the pH Combined Electrode Sensor in accordance with the sensor input specifications of the WIL-102-PH.
- Keep the input wires and power lines separate.

Note about the pH Combined Electrode Sensor Cable

The pH Combined Electrode Sensor cable is a highly-insulated (electrical) cable. Please handle it with utmost care as follows.

- Do not allow terminals and socket of the pH Combined Electrode Sensor cable to come in contact with moisture or oil of any kind. Likewise, ensure fingers are clean, otherwise the insulation will deteriorate, resulting in unstable indication.
Be sure to keep the cable dry and clean at all times.
If the cable is stained, clean it with alcohol, and dry it completely.
- For calibration or electrode checking/replacement, the pH Combined Electrode Sensor cable should be wired with sufficient length.
- Keep the pH Combined Electrode Sensor cable and junction cable away from electrical devices, such as motors or their power lines from which inductive interference emanates.

Connection

The pH Combined Electrode Sensor cable has the following terminals.

| Code | Terminal |
|---------|---|
| G | Glass electrode terminal |
| R | Reference electrode terminal |
| T, T | Temperature compensation electrode terminals (Cu500) |
| A, B | Temperature compensation electrode terminals [Pt100 (2-wire), Pt1000] |
| A, B, B | Temperature compensation electrode terminals [Pt100 (3-wire)] |
| E | Shield wire terminal |

For the pH Combined Electrode Sensor with No Temperature Compensation, T, T or A, B, B cables are not available.

E cables are available depending on the sensor type.

During operation, the pH/Temperature Display may become abnormal or unstable due to inductive interference or noise. In this case, try [Grounding of shield wire terminal (E) (P.78)].

3. Operation and Maintenance Precautions



Caution

- Do not touch live terminals. This may cause an electrical shock or problems in operation.
- Turn the power supply to the instrument OFF when retightening the terminal or cleaning.
Working on or touching the terminal with the power switched ON may result in severe injury or death due to electrical shock.
- Use a soft, dry cloth when cleaning the instrument.
(Alcohol based substances may tarnish or deface the unit.)
- As the display section is vulnerable, be careful not to put pressure on, scratch or strike it with a hard object.

Contents

| | |
|--|----|
| 1. Model | 7 |
| 1.1 Model | 7 |
| 1.2 How to Read the Model Label | 7 |
| 2. Name and Functions of Instrument | 8 |
| 3. Mounting to the Control Panel | 9 |
| 3.1 Site Selection | 9 |
| 3.2 External Dimensions (Scale: mm) | 9 |
| 3.3 Mounting | 9 |
| 4. Removal | 11 |
| 5. Wiring | 12 |
| 5.1 Lead Wire Solderless Terminal | 13 |
| 5.2 Terminal Arrangement | 13 |
| 5.3 Wire the Communication Line | 14 |
| 6. Outline of Key Operation and Setting Groups | 16 |
| 6.1 Outline of Key Operation | 16 |
| 6.2 Setting Groups | 16 |
| 7. Key Operation Flowchart | 18 |
| 8. Setup | 20 |
| 8.1 Turn the Power Supply to the WIL-102-PH ON | 20 |
| 8.2 pH Input Group | 20 |
| 8.3 Temperature Input Group | 28 |
| 8.4 Basic Function Group | 29 |
| 8.5 Zero/Slope Indication Group | 37 |
| 9. Calibration | 38 |
| 9.1 pH Calibration Mode | 38 |
| 9.1.1 Automatic Calibration | 38 |
| 9.1.2 Manual Calibration | 40 |
| 9.1.3 Error Code during pH Calibration | 41 |
| 9.2 Temperature Calibration Mode | 42 |
| 9.3 Transmission Output 1 Adjustment Mode | 43 |
| 9.4 Transmission Output 2 Adjustment Mode | 44 |
| 10. Measurement | 45 |
| 10.1 Starting Measurement | 45 |
| 10.2 A□□ Output | 45 |
| 10.3 pH Input Error Alarm | 46 |
| 10.4 Error Output | 46 |
| 10.5 Fail Output | 46 |
| 10.6 Cleansing Output | 46 |
| 10.7 Manual Cleansing Mode | 47 |
| 10.8 Error Code during Measurement | 48 |
| 10.9 Transmission Output 1 and 2 | 48 |
| 10.10 pH Fluctuation Alarm Output | 48 |
| 11. Communication | 49 |
| 11.1 System Configuration Example | 49 |
| 11.2 Setting Method of the pH Meter | 49 |
| 11.3 Communication Procedure | 50 |
| 11.4 Shinko Protocol | 51 |
| 11.4.1 Transmission Mode | 51 |
| 11.4.2 Command Configuration | 51 |
| 11.4.3 Checksum Calculation | 52 |

| | |
|--|----|
| 11.5 MODBUS Protocol | 53 |
| 11.5.1 Transmission Mode..... | 53 |
| 11.5.2 Data Communication Interval..... | 53 |
| 11.5.3 Message Configuration | 53 |
| 11.5.4 Message Example | 55 |
| 11.6 Communication Command Table..... | 57 |
| 11.6.1 Notes about Setting/Reading Command..... | 57 |
| 11.6.2 Setting/Reading Command..... | 58 |
| 11.6.3 Read Only Command | 64 |
| 11.7 pH Calibration, Transmission Output 1 and 2 Adjustment via Communication Command..... | 66 |
| 11.7.1 pH Calibration | 66 |
| 11.7.2 Transmission Output 1 Adjustment..... | 68 |
| 11.7.3 Transmission Output 2 Adjustment..... | 68 |
| 11.8 Notes on Programming Monitoring Software..... | 69 |
| 11.8.1 How to Speed up the Scan Time | 69 |
| 11.8.2 How to Read the Set Value Changes Made by Front Keypad Operation..... | 69 |
| 11.8.3 Note when Sending All Set Values Simultaneously | 69 |
| 12. Specifications | 70 |
| 12.1 Standard Specifications | 70 |
| 12.2 Optional Specifications..... | 75 |
| 13. Troubleshooting..... | 77 |
| 13.1 Indication..... | 77 |
| 13.2 Key Operation | 78 |
| 13.3 Communication | 79 |
| 14. Character Tables | 80 |

1. Model

1.1 Model

| | | | | | |
|----------------------|----|-----|--|------------------------------|--|
| WIL-10 | 2 | -PH | | , □□□ | |
| Input Points | 2 | | | | 2 points |
| Input | PH | | | pH Combined Electrode Sensor | Pt spec (*1) |
| | | | | | Pt1000 |
| | | | | | Pt100 |
| | | | | Cu spec (*1) | Cu500/25°C |
| Power Supply Voltage | 1 | | | | 100 to 240 V AC (standard) |
| | | | | | 24 V AC/DC (*2) |
| Option | | | | EVT | A□□ output (A11, A12, A21, A22) |
| | | | | TA | Transmission output 1 (*3) |
| | | | | TA2 | Transmission output 1, Transmission output 2 |

(*1) This input temperature specification was specified at the time of ordering.

(*2) Power supply voltage 100 to 240 V AC is standard.


When ordering 24 V AC/DC, enter "1" in Power Supply Voltage after "PH".

(*3) If the TA option is ordered, the EVT option (A1 output only) will be automatically added.

1.2 How to Read the Model Label


The model label is attached to the left side of the case.

- Label on the left side of the case

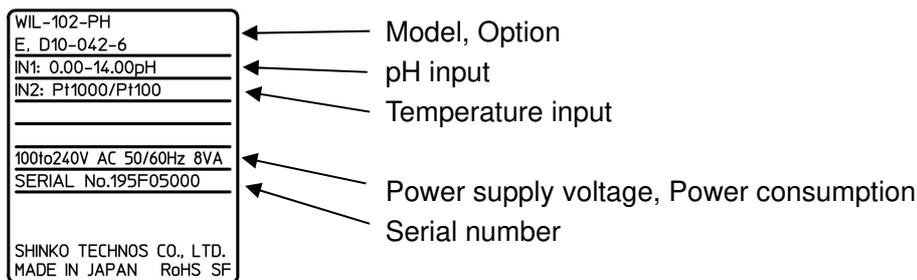

(Fig. 1.2-1)

2. Name and Functions of Instrument

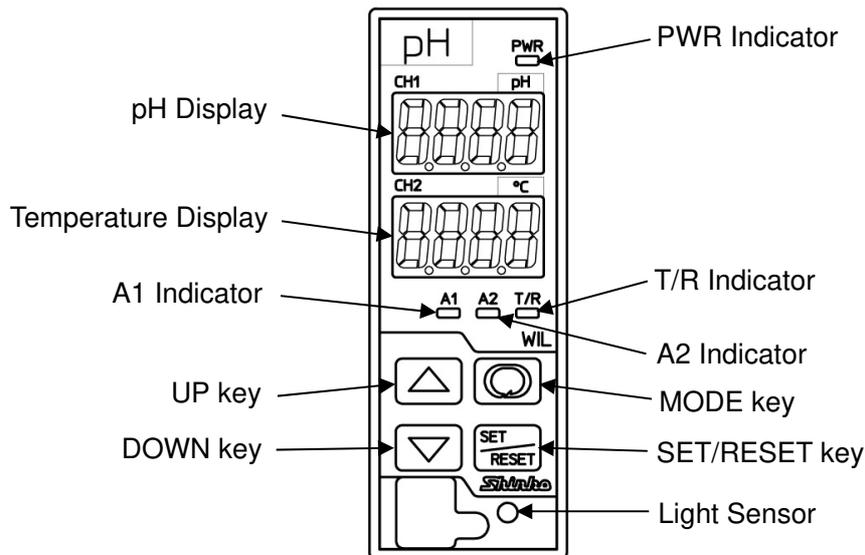

(Fig. 2-1)

Displays

| | |
|---------------------|--|
| pH Display | pH or characters in setting mode are indicated in red. Indications differ depending on the selections in [Display selection (p.32)]. |
| Temperature Display | Temperature or values in setting mode are indicated in red. Indications differ depending on the selections in [Display selection (p.32)]. |

Action Indicators

| | |
|---------------|---|
| PWR Indicator | When power supply to the instrument is turned ON, the yellow LED is lit. |
| A1 Indicator | When A1 output (Contact output 1) is ON, the red LED lights. (Turns OFF if TA2 option is added.) |
| A2 Indicator | When A2 output (Contact output 2) is ON, the yellow LED lights. (Turns OFF if TA option or TA2 option is added.) |
| T/R Indicator | The yellow LED lights during Serial communication TX output (transmitting). |

Keys

| | |
|---|--|
|  UP key | Increases the numeric value. |
|  DOWN key | Decreases the numeric value. |
|  MODE key | Selects a setting group. |
|  SET/RESET key | Switches the setting modes, and registers the set value. |

| | |
|--------------|--|
| Light Sensor | Automatically measures and controls brightness of the pH Display, Temperature Display and Action indicators. |
|--------------|--|

Notice

When setting the specifications and functions of this instrument, connect mains power cable to terminals 13 and 14 first, then set them referring from “6. Outline of Key Operation and Setting Groups” to “8. Setup (pp.16 to 37)” before performing “3. Mounting to the Control Panel (p.9)” and “5. Wiring (p.12)”.

3. Mounting to the Control Panel

3.1 Site Selection



Caution

Use within the following temperature and humidity ranges.

Temperature: 0 to 50°C (32 to 122°F) (No icing), Humidity: 35 to 85 %RH (Non-condensing)


If the WIL-102-PH is installed within a control panel, the ambient temperature of the unit – not the ambient temperature of the control panel – must be kept under 50°C. Otherwise the life of electronic parts (especially electrolytic capacitors) of the unit will be shortened.

This instrument is intended to be used under the following environmental conditions (IEC61010-1): Overvoltage category II, Pollution degree 2

Ensure the mounting location corresponds to the following conditions:

- A minimum of dust, and an absence of corrosive gases
- No flammable, explosive gases
- No mechanical vibrations or shocks
- No exposure to direct sunlight, an ambient temperature of 0 to 50°C (32 to 122°F) that does not change rapidly
- An ambient non-condensing humidity of 35 to 85 %RH
- No large capacity electromagnetic switches or cables through which a large current is flowing
- No water, oil, chemicals or the vapors of these substances can come into direct contact with the unit


3.2 External Dimensions (Scale: mm)

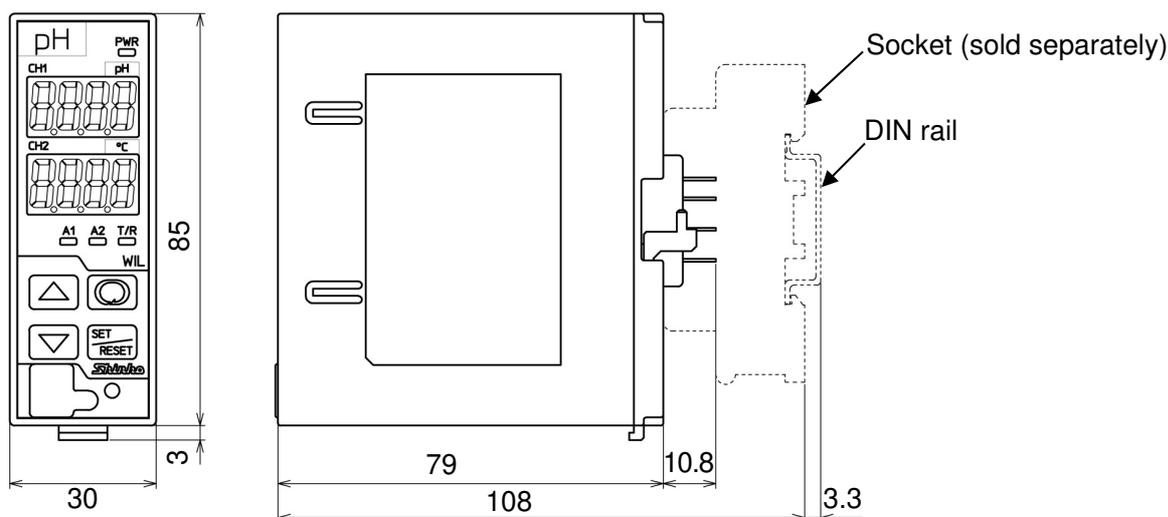

(Fig. 3.2-1)

3.3 Mounting

(1) Hook the upper part of the socket on the DIN rail, and mount it (A clicking sound is heard).

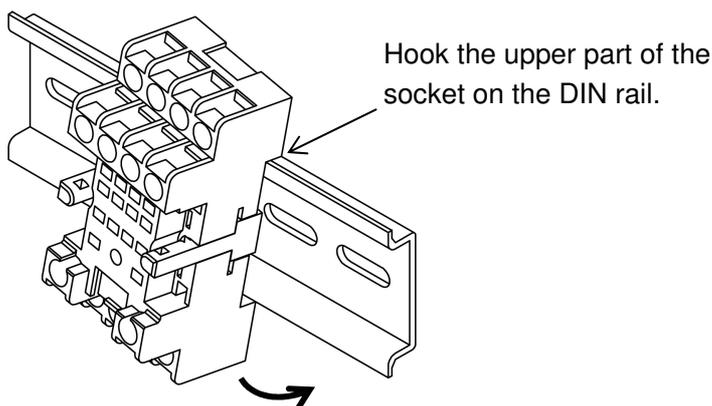


(Fig. 3.3-1)

Caution


Before inserting the WIL-102-PH into the socket, wire the unit while referring to Section “5. Wiring” (p.12).

(2) Check that the Lock Release has been lowered.

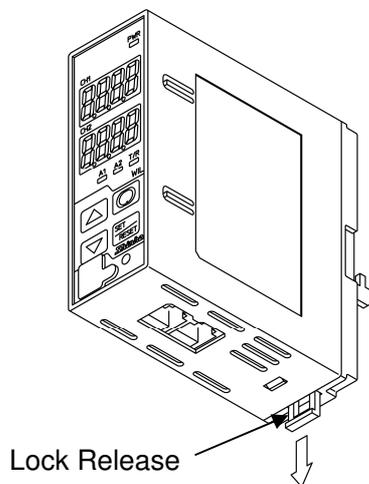


(Fig. 3.3-2)

(3) Insert the WIL-102-PH into the socket.

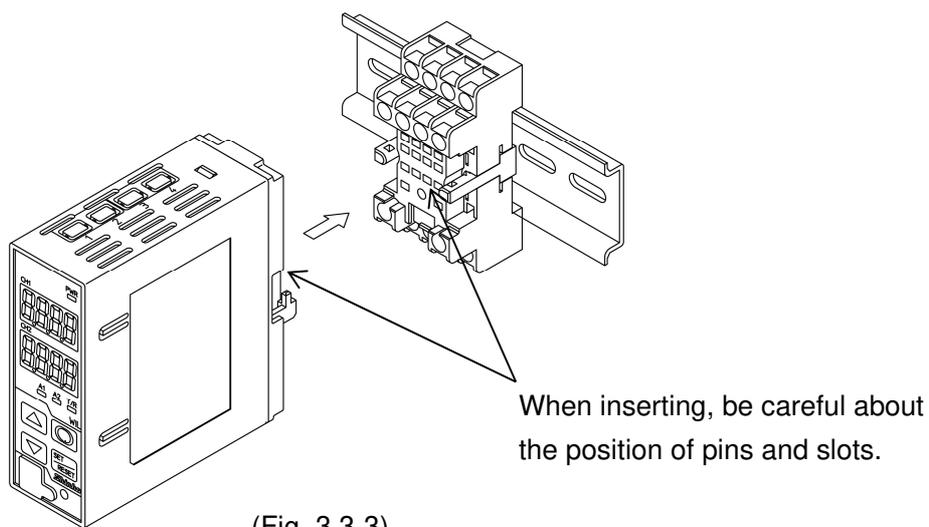

(Fig. 3.3-3)

(4) Fix the WIL-102-PH and the socket by pushing the Lock Release up.

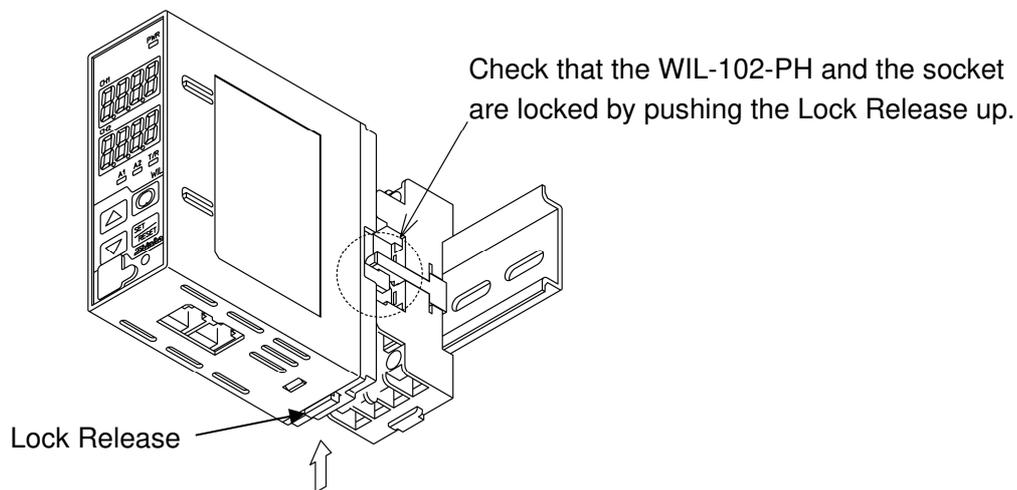


(Fig. 3.3-4)

4. Removal


(1) Turn the power supply to the unit OFF.

(2) Pull the Lock Release down, and release the WIL-102-PH from the socket.

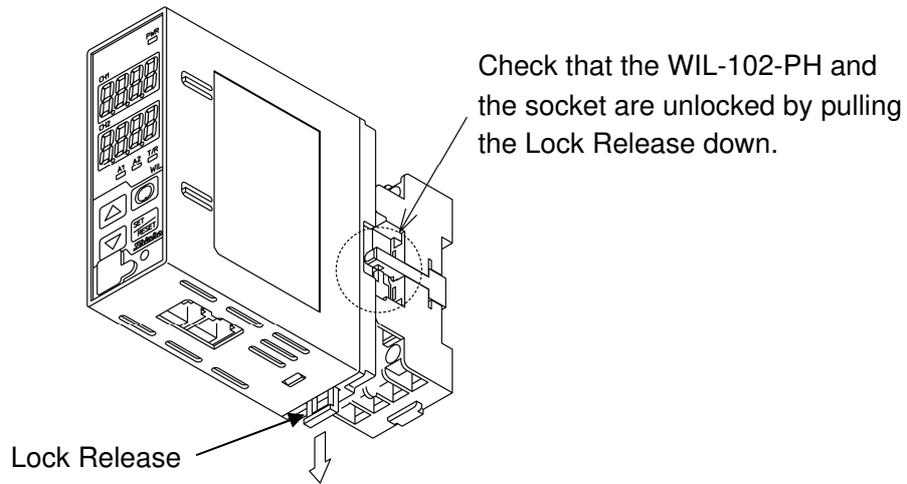


(Fig. 4-1)

(3) Separate the WIL-102-PH from the socket.

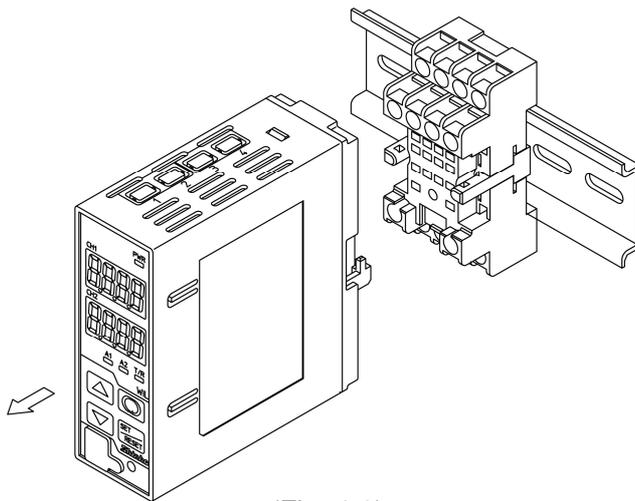

(Fig. 4-2)

(4) Remove the socket from the DIN rail by pulling the socket Lock Release (at the bottom of the socket) down.

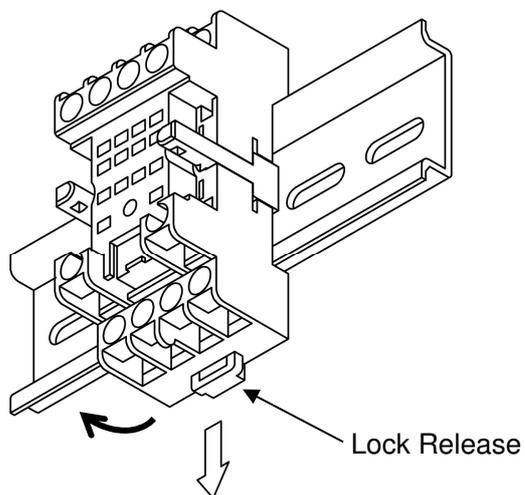

(Fig. 4-3)

5. Wiring

Warning

Turn the power supply to the instrument off before wiring or checking.

Working on or touching the terminal with the power switched on may result in severe injury or death due to electrical shock.

Caution

- Do not leave wire remnants in the instrument, as they could cause a fire or a malfunction.
- Use a solderless terminal with an insulation sleeve in which the M3 screw fits when wiring the unit.
- Tighten the terminal screw using the specified torque. If excessive force is applied to the screw when tightening, the terminal screw may be damaged.
- This instrument does not have a built-in power switch, circuit breaker and fuse. It is necessary to install a power switch, circuit breaker and fuse near the instrument. (Recommended fuse: Time-lag fuse, rated voltage 250 V AC, rated current 2 A)
- For a 24 V AC/DC power source, do not confuse polarity when using direct current (DC).
- Do not apply a commercial power source to the sensor which is connected to the input terminal nor allow the power source to come into contact with the sensor.
- Use the pH Combined Electrode Sensor in accordance with the sensor input specifications of this unit.
- Keep the input wires and power lines separate.

Note about the pH Combined Electrode Sensor Cable

The pH Combined Electrode Sensor cable is a highly-insulated (electrical) cable. Please handle it with utmost care as follows.

- Do not allow terminals and socket of the pH Combined Electrode Sensor cable to come in contact with moisture or oil of any kind. Likewise, ensure fingers are clean, otherwise the insulation will deteriorate, resulting in unstable indication. Be sure to keep the cable dry and clean at all times. If the cable is stained, clean it with alcohol, and dry it completely.
- For calibration or electrode checking/replacement, the pH Combined Electrode Sensor cable should be wired with sufficient length. Keep the pH Combined Electrode Sensor cable and junction cable away from electrical devices, such as motors or their power lines from which inductive interference emanates.

Connection

The pH Combined Electrode Sensor cable has the following terminals.

| Code | Terminal |
|---------|---|
| G | Glass electrode terminal |
| R | Reference electrode terminal |
| T, T | Temperature compensation electrode terminals (Cu500) |
| A, B | Temperature compensation electrode terminals [Pt100 (2-wire), Pt1000] |
| A, B, B | Temperature compensation electrode terminals [Pt100 (3-wire)] |
| E | Shield wire terminal |

For the pH Combined Electrode Sensor with No Temperature Compensation, T, T or A, B, B cables are not available.


E cables are available depending on the sensor type.

During operation, the pH/Temperature Display may become abnormal or unstable due to inductive interference or noise. In this case, try [Grounding of shield wire terminal (E) (P.78)].

5.1 Lead Wire Solderless Terminal


Use a solderless terminal with an insulation sleeve in which an M3 screw fits as follows.
The tightening torque should be 0.63 N•m.

| Solderless Terminal | Manufacturer | Model |
|---------------------|---------------------------------------|--------------|
| Y-type | Nichifu Terminal Industries CO., LTD. | TMEV1.25Y-3S |

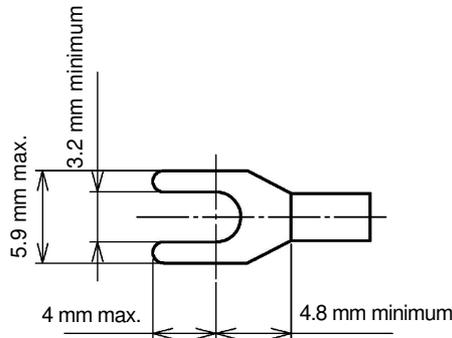

(Fig. 5.1-1)

5.2 Terminal Arrangement

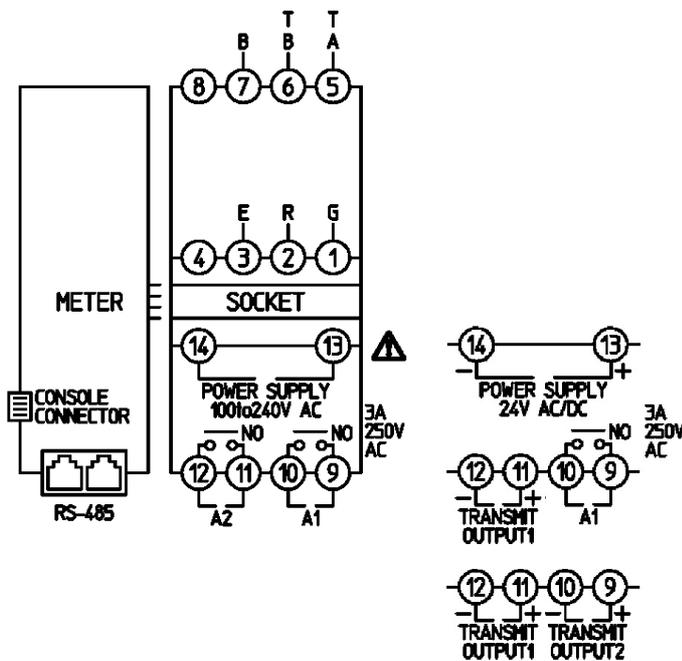

Modular Jack Pin (WIL-102-PH side arrangement)

| | | | |
|--------|--|-------|-------|
| No. 1 | | No. 1 | COM |
| No. 6 | | No. 2 | NC |
| No. 1 | | No. 3 | YB(+) |
| No. 6 | | No. 4 | YA(-) |
| RS-485 | | No. 5 | NC |
| | | No. 6 | COM |

(Fig. 5.2-1)


- G, R: Electrode sensor terminals (①-②)
pH Combined Electrode Sensor
 - E: Shield wire terminal (③)
pH Combined Electrode Sensor
 - T, T: Temperature compensation sensor terminals (⑤-⑥)
Temperature element: Cu500 (2-wire)
 - A, B: Temperature compensation sensor terminals (⑤-⑥)
Temperature element: Pt100 (2-wire), Pt1000
 - A, B, B: Temperature compensation sensor terminals (⑤-⑥-⑦)
Temperature element: Pt100 (3-wire)
- When the EVT option is ordered
- A1: A1 output terminals (⑨-⑩)
 - A2: A2 output terminals (⑪-⑫)
- When the TA option is ordered
- A1: A1 output terminals (⑨-⑩)
 - TRANSMISSION OUTPUT1: Transmission output 1 terminals (⑪-⑫)
- When the TA2 option is ordered
- TRANSMISSION OUTPUT2: Transmission output 2 terminals (⑨-⑩)
 - TRANSMISSION OUTPUT1: Transmission output 1 terminals (⑪-⑫)
- POWER SUPPLY: Power terminals (⑬-⑭)
24 V AC/DC (Enter "1" after the input code.)
- RS-485: Serial Communication modular jack

When no option is ordered, A1, A2, TRANSMIT OUTPUT1 and TRANSMIT OUTPUT2 terminals are not equipped.

5.3 Wire the Communication Line


Connect to the modular jack at the bottom of the instrument, using CDD or CPP (sold separately).

- **Wiring Example Using USB communication cable CMC-001-3 (sold separately)**

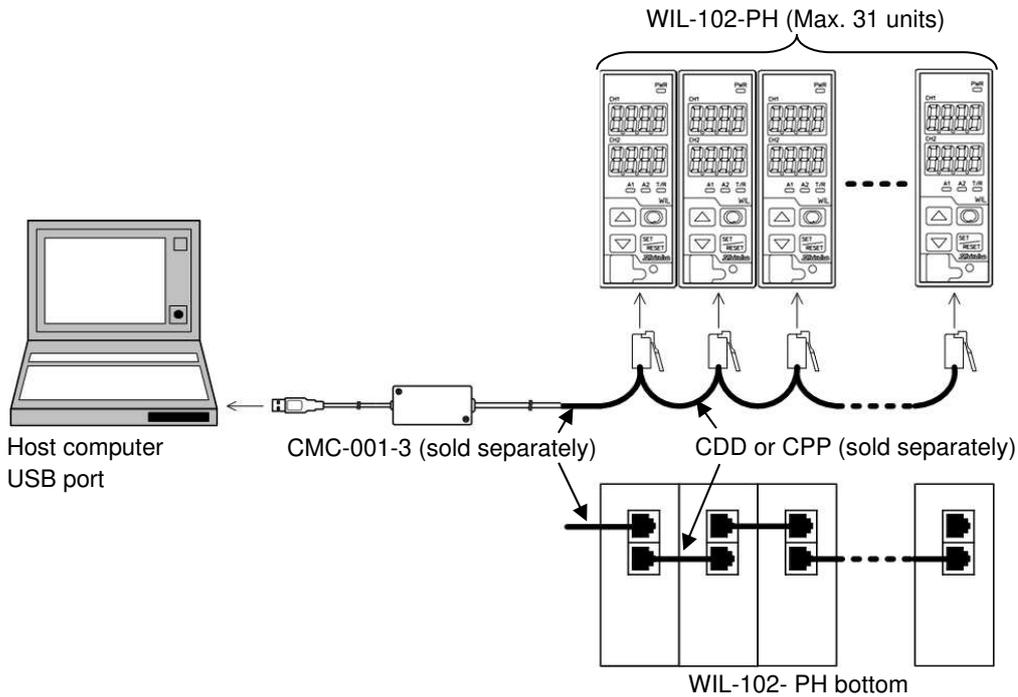

(Fig. 5.3-1)

- **Wiring Example Using a Communication Converter IF-400**

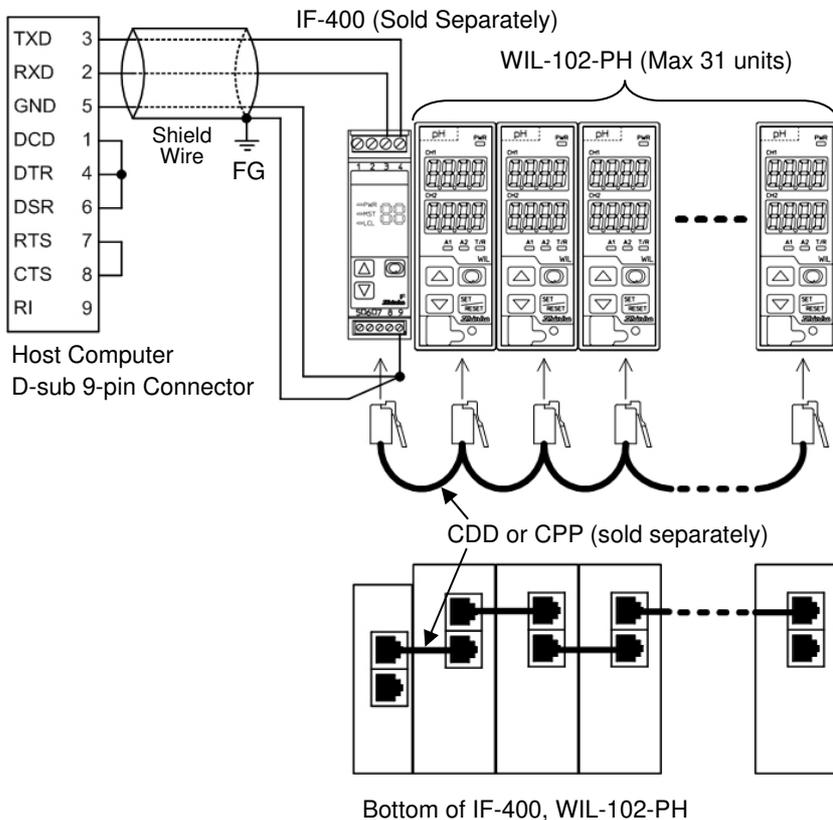

(Fig. 5.3-2)

Shield Wire

Be sure to ground only one end of the shield wire so that current cannot flow to the shield wire.

If both ends of the shield wire are grounded, the circuit will be closed, resulting in a ground loop. This may cause noise.

Be sure to ground the FG.

Recommended cable: OTSC-VB 2PX0.5SQ (made by Onamba Co., Ltd.) or equivalent
(Use a twisted pair cable.)

Terminator (Terminal Resistor)

The terminator is mounted at the end of the wire when connecting multiple peripheral devices to a personal computer. The terminator prevents signal reflection and disturbance.

Do not connect a terminator with the communication line because each WIL-102-PH has built-in pull-up and pull-down resistors.


Communication converter IF-400 (sold separately) has a built-in terminal resistor.

6. Outline of Key Operation and Setting Groups

6.1 Outline of Key Operation

Setting items are divided into groups, and group selection has to be made with keypads. Press the  key in pH/Temperature Display Mode, or Cleansing Output Mode. The unit enters Group Selection mode. Select a group with the , and press the . The unit enters each setting item. To set each setting item, use the  or  key, and register the set value with the  key.

6.2 Setting Groups

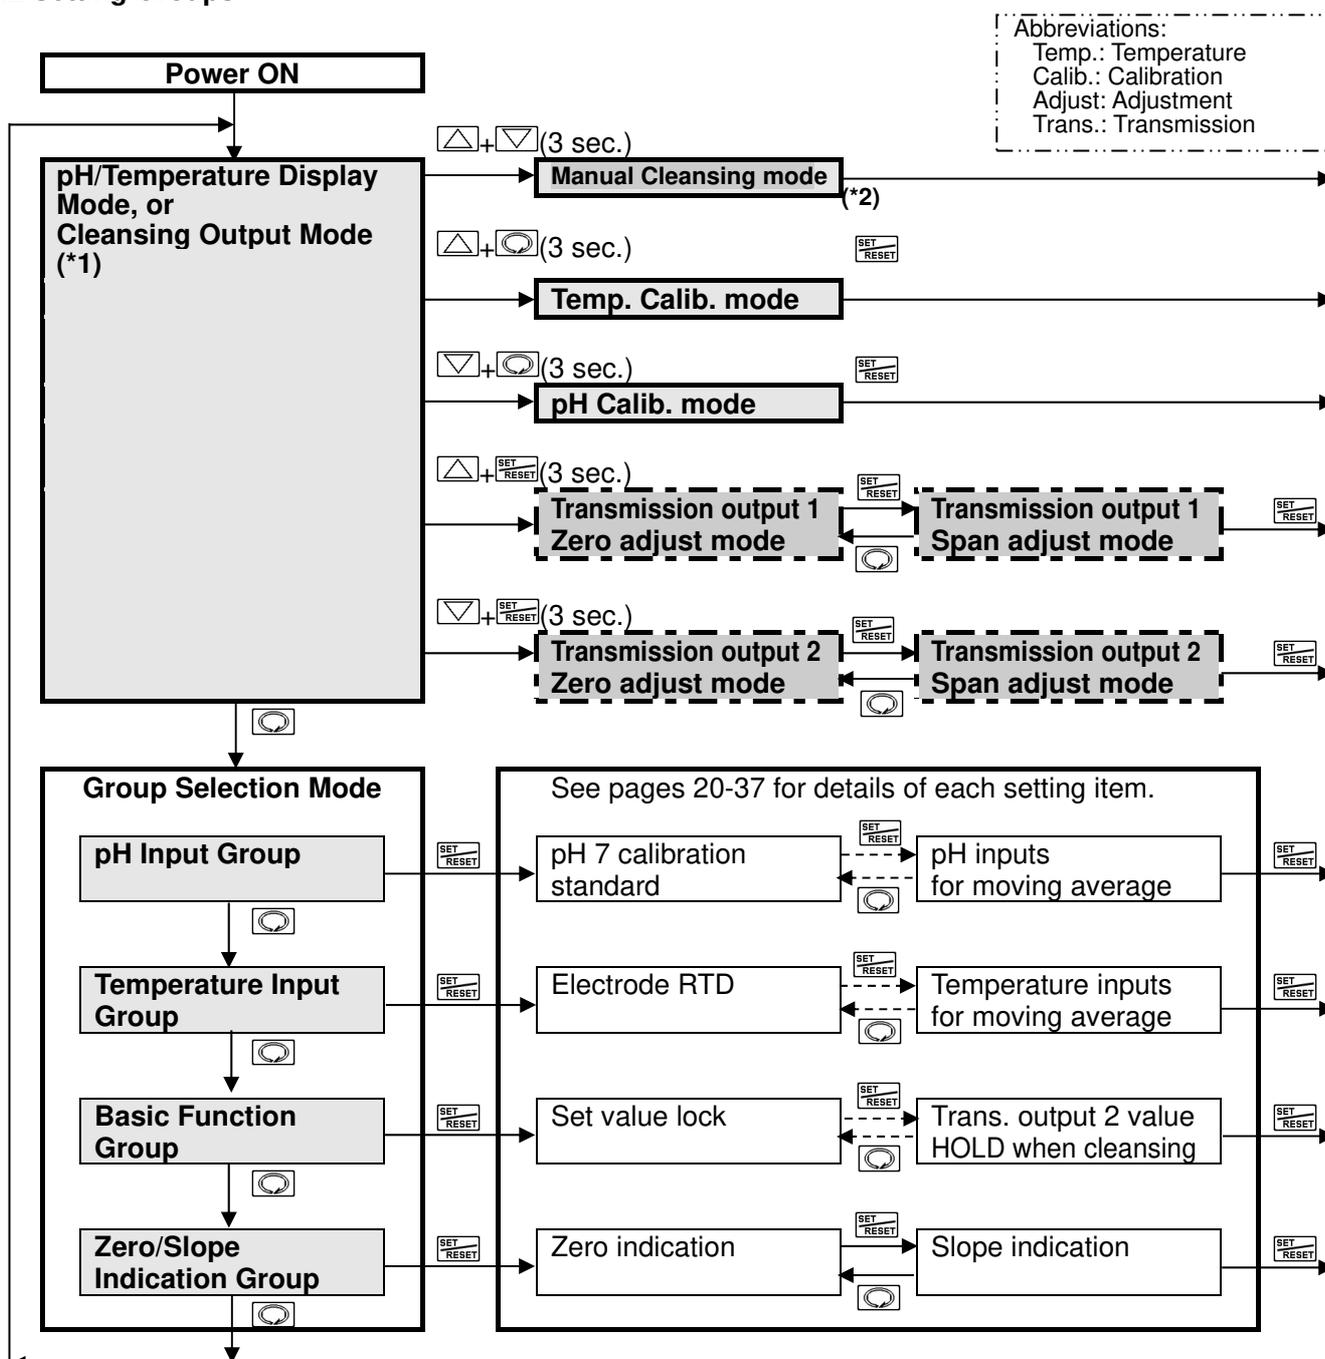

(*1) During pH/Temperature Display Mode, or Cleansing Output Mode, indicates the item selected in [Display selection (p.32)]. If power is turned ON again, the last mode (pH/Temperature Display Mode, or Cleansing Output Mode) at power OFF will resume.

(*2) If  (Cleansing output) is selected in [A11, A12, A21, A22 type], the unit can enter Manual Cleansing mode. After cleansing action is complete, the unit automatically reverts to Cleansing Output Mode.




Available only when the TA or TA2 option is ordered.

About Key Operation

- + (3 sec): Press and hold the key and key (in that order) together for 3 seconds.
The unit will proceed to Manual Cleansing mode.
- + (3 sec): Press and hold the key and key (in that order) together for 3 seconds.
The unit will proceed to Temperature calibration mode.
- + (3 sec): Press and hold the key and key (in that order) together for 3 seconds.
The unit will proceed to pH calibration mode.
- + (3 sec): Press and hold the key and key (in that order) together for 3 seconds.
The unit will proceed to Transmission output 1 Zero adjustment mode.
- + (3 sec): Press and hold the key and key (in that order) together for 3 seconds.
The unit will proceed to Transmission output 2 Zero adjustment mode.
- or : Press the or key. The unit will proceed to the next setting item, illustrated by an arrow.
- or : Press the or key multiple times until the desired setting mode appears.
- To revert to pH/Temperature Display Mode, or Cleansing Output Mode, press and hold the key for 3 seconds while in any mode.

7. Key Operation Flowchart

Abbreviations:
H/L: High/Low
Temp.: Temperature

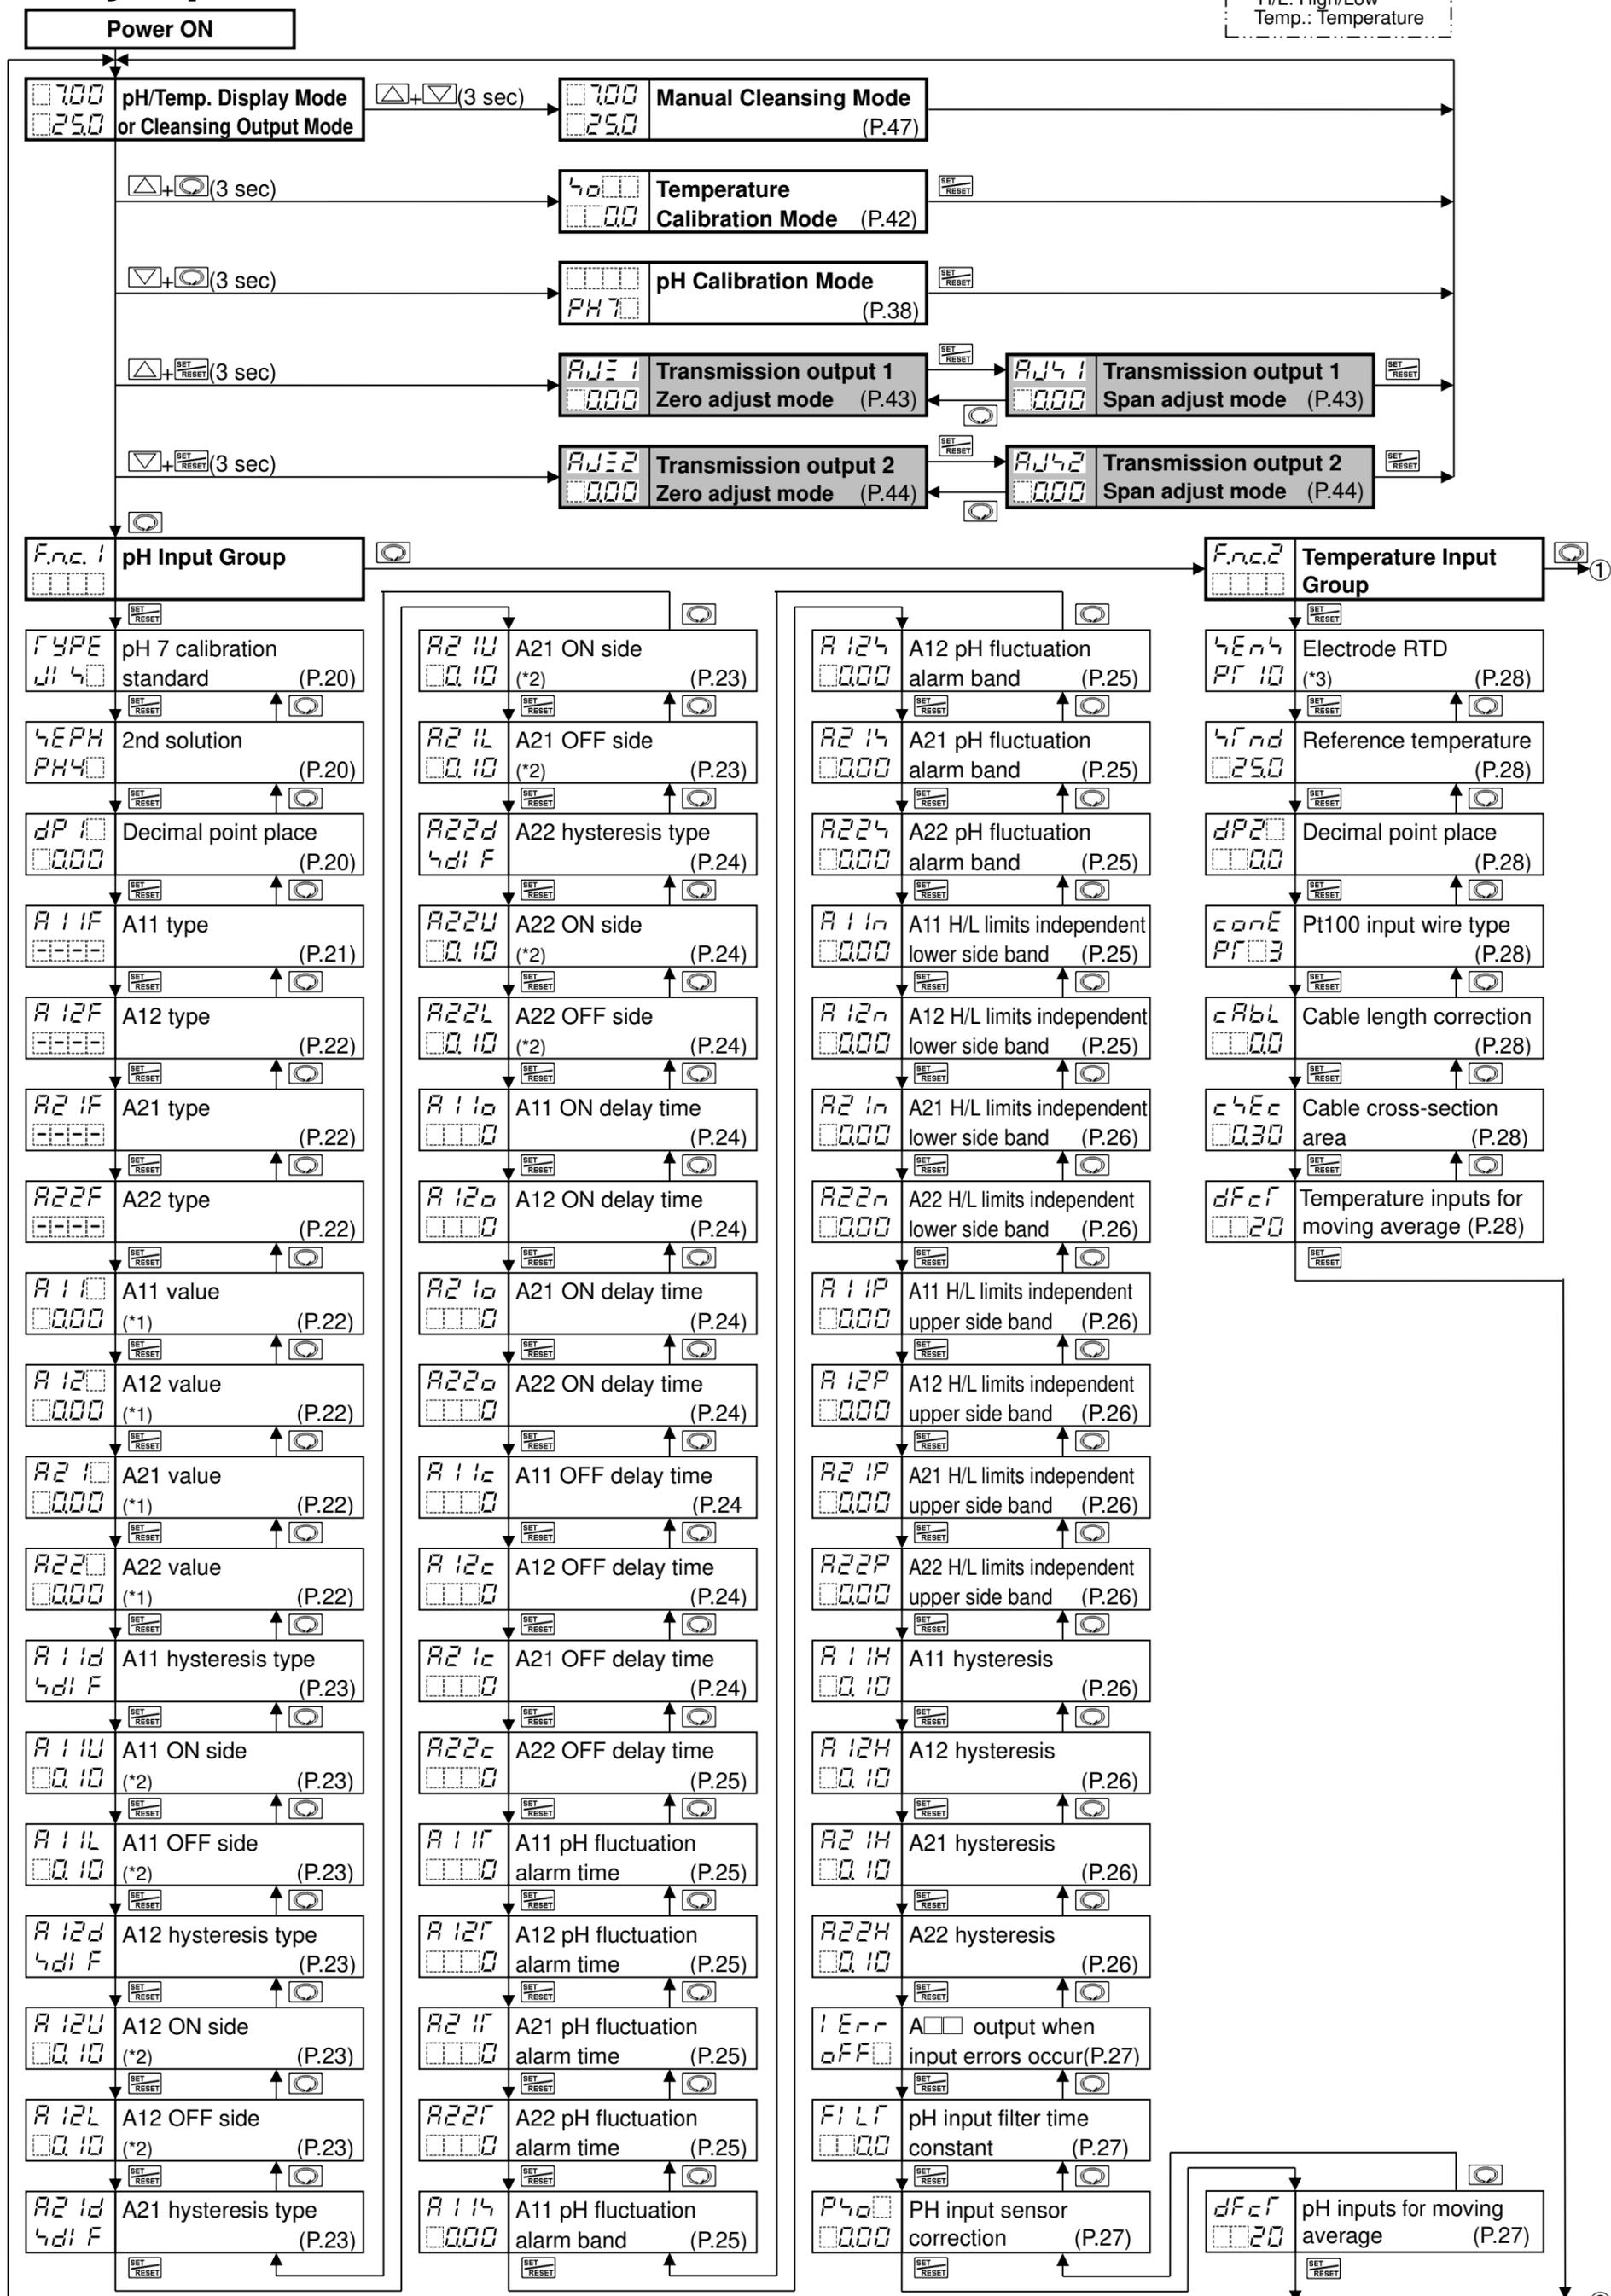

● **About Setting Items**


| | |
|---------|-----------------------------------|
| TYPE | pH 7 calibration standard (P.20) |
| Trans 1 | Transmission output 1 type (P.30) |

- **Upper left:** pH Display: Indicates the setting item characters.
 - **Lower left:** Temperature Display: Indicates the factory default.
 - **Right side:** Indicates the setting item and reference page.
- Setting item in shaded section will be displayed only when the corresponding option is ordered.
 If the TA option is added, A2 related setting items are not available.
 If the TA2 option is added, A1 and A2 related setting items are not available.

(*1): Factory default value is different depending on the A□□ type selection. pH input: pH 0.00, Temperature input: 0.0°C
 (*2): Factory default value is different depending on the A□□ type selection. pH input: pH 0.10, Temperature input: 1.0°C
 (*3): Factory default value is different depending on the input spec. Pt spec: PFI□, Cu spec: cUS□

● **About Key Operation**

- $\triangle + \nabla$ (3 sec): Press and hold the \triangle , ∇ keys (in that order) for 3 sec. The unit enters Manual Cleansing mode.
- $\triangle + \text{SET/RESET}$ (3 sec): Press and hold the \triangle , SET/RESET keys (in that order) for 3 sec. The unit enters Temperature calibration mode.
- $\nabla + \text{SET/RESET}$ (3 sec): Press and hold the ∇ , SET/RESET keys (in that order) for 3 sec. The unit enters pH calibration mode.
- $\triangle + \text{SET/RESET}$ (3 sec): Press and hold the \triangle , SET/RESET keys (in that order) for 3 sec. The unit enters Transmission output 1 Zero adjustment mode.
- $\nabla + \text{SET/RESET}$ (3 sec): Press and hold the ∇ , SET/RESET keys (in that order) for 3 sec. The unit enters Transmission output 2 Zero adjustment mode.
- SET/RESET or SET/RESET : Press the SET/RESET or SET/RESET key. The unit enters the next setting item.
- To revert to pH/Temperature Display Mode, or Cleansing Output Mode, press and hold the SET/RESET key for 3 sec while in any mode.

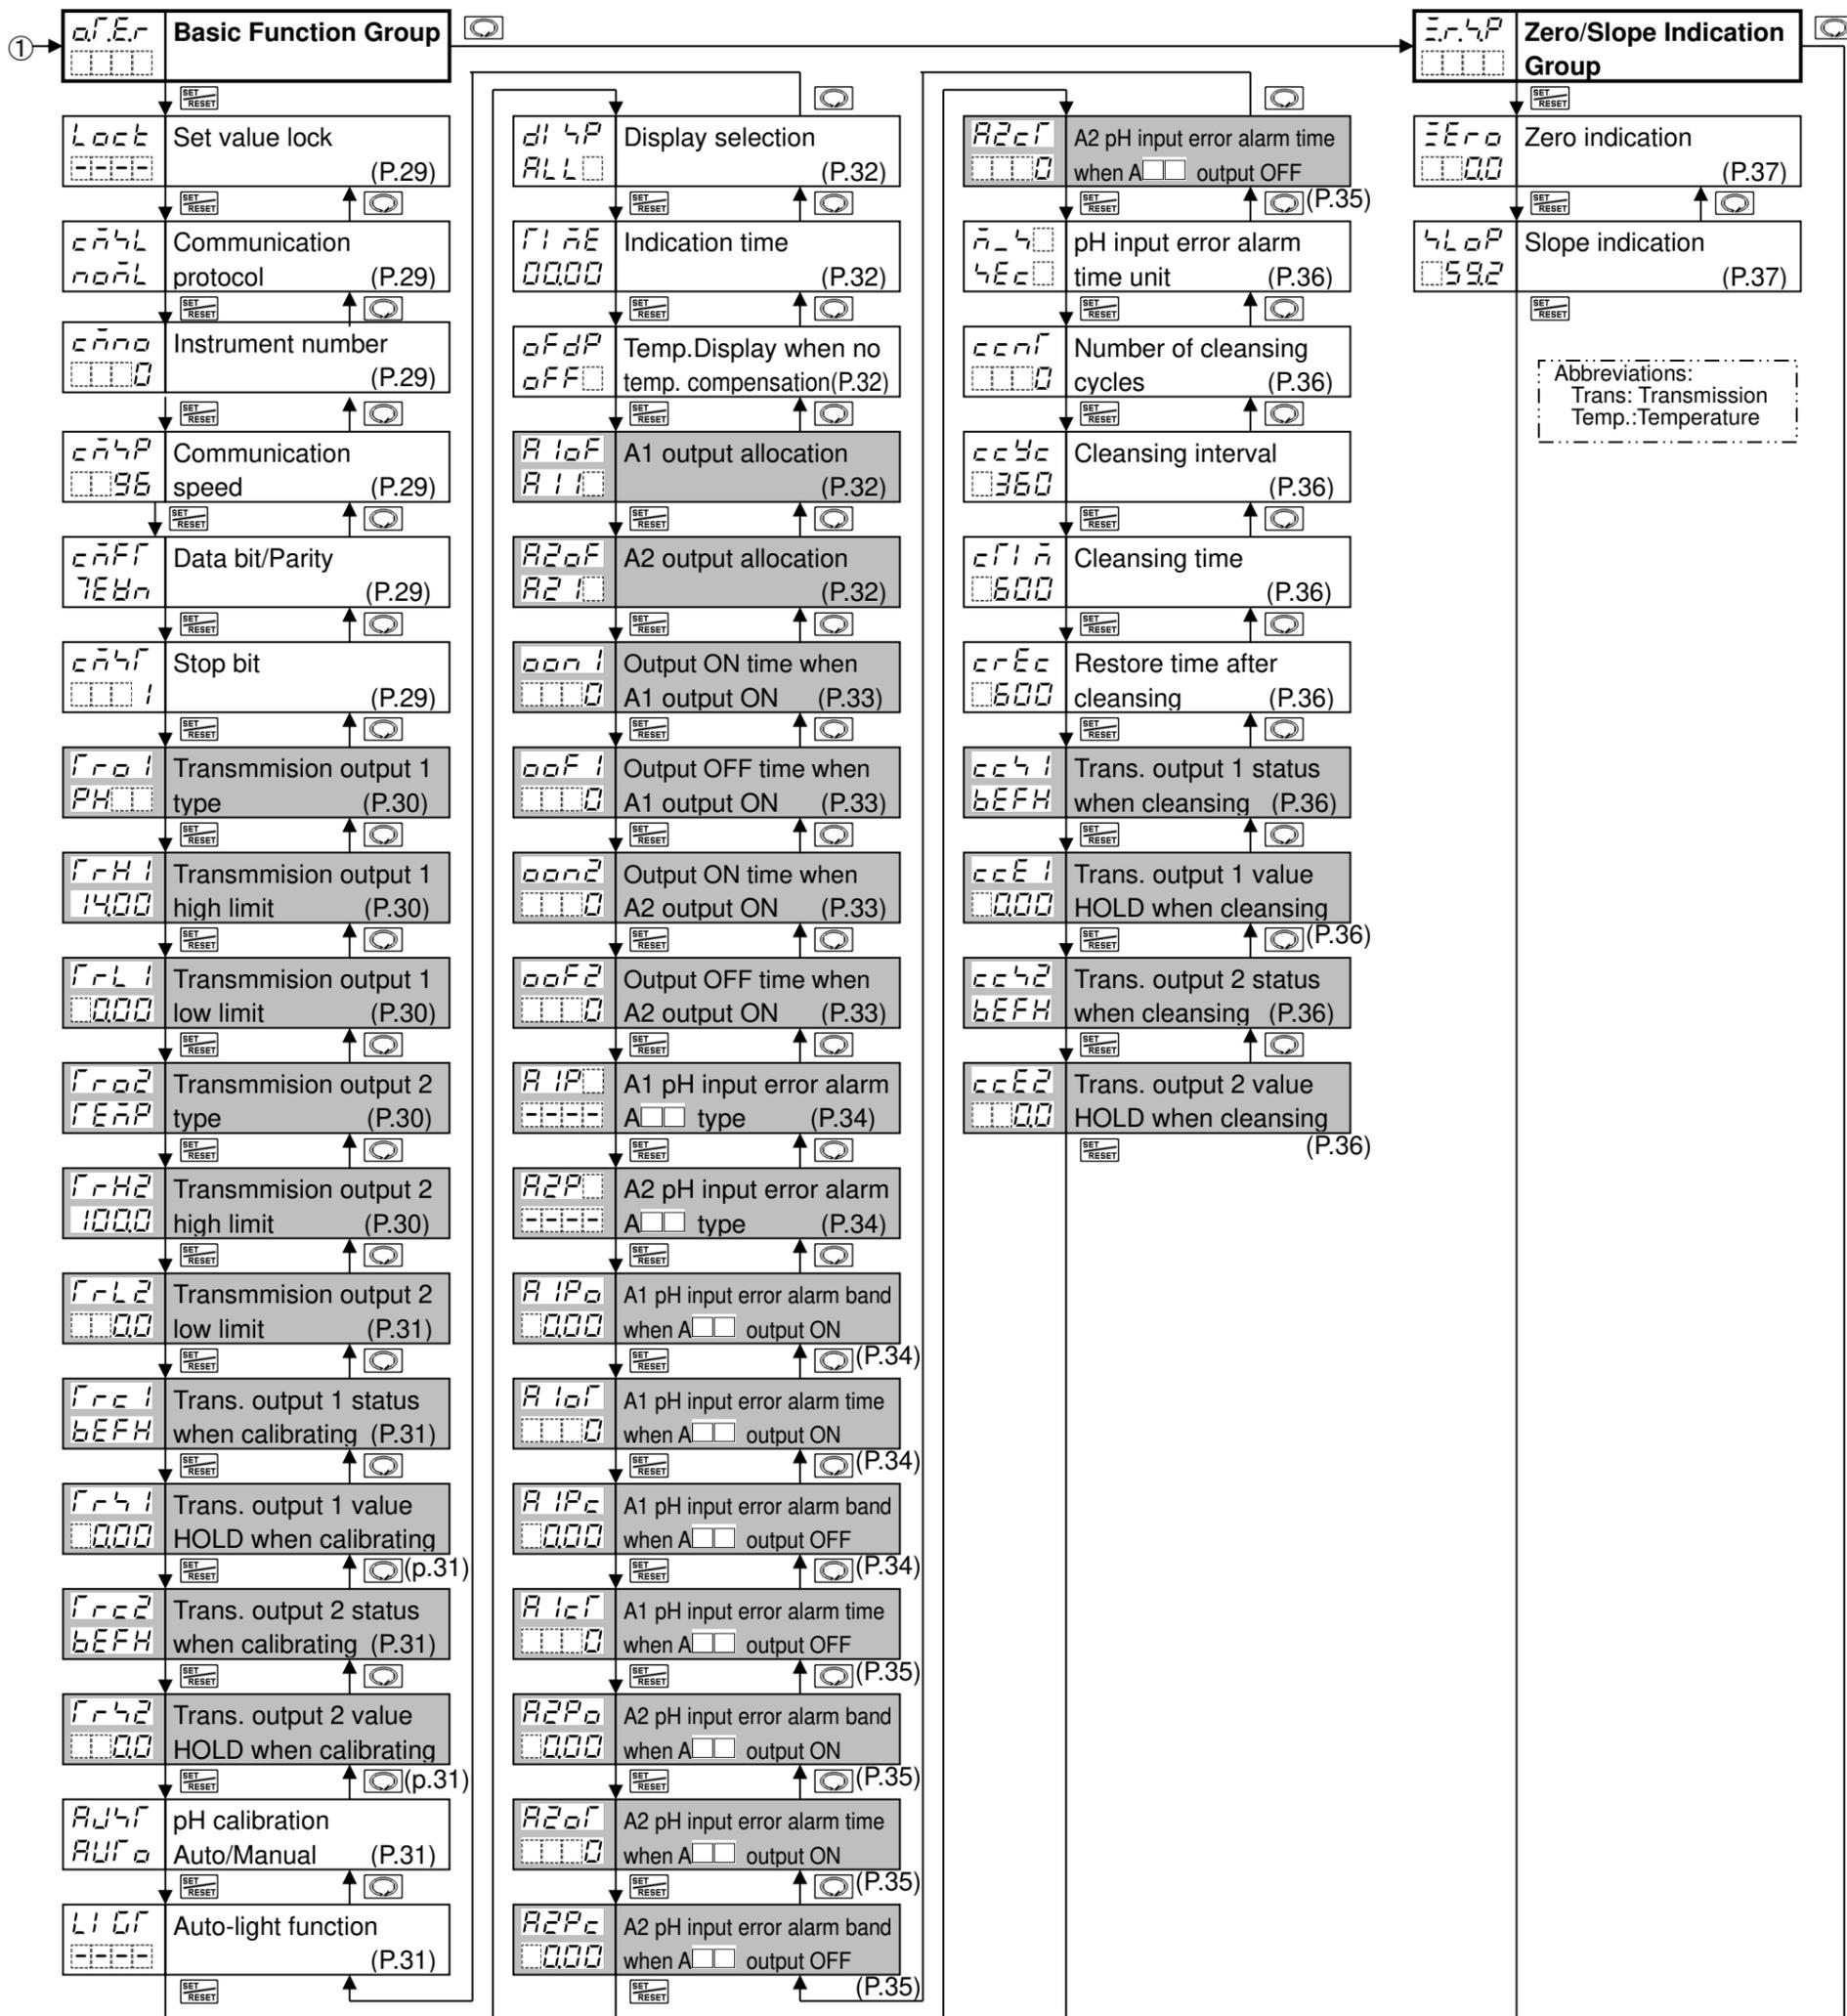

8. Setup

Setup should be done before using this instrument, according to the user's conditions:

Setting the 2nd Solution, A11, A12, A21, A22 types, Electrode RTD, Communication, pH Calibration Auto/Manual, etc.

Setup can be conducted in the pH Input group, Temperature Input Group and Basic Function Group.

If the user's specification is the same as the factory default of the WIL-102-PH, or if setup has already been completed, it is not necessary to set up the instrument. Proceed to Section "9. Calibration (p.38)".

8.1 Turn the Power Supply to the WIL-102-PH ON.

For approx. 4 seconds after the power is switched ON, the input characters are indicated on the pH Display and Temperature Display.

Depending on the input specification, indication on the Temperature Display differs as follows.

Pt spec

| pH Display | Temperature Display | Item selected in [Electrode RTD (p.28)] | Item selected in [Pt100 input wire type (p.28)] |
|------------|---------------------|---|---|
| PH□□ | Unlit | none : No temperature compensation | |
| | PT 10 | PT 10 : Pt1000 | |
| | PT 02 | PT 10 : Pt100 | PT 02 : 2-wire type |
| | PT 03 | | PT 03 : 3-wire type |

Cu spec

| pH Display | Temperature Display | Item selected in [Electrode RTD (p.28)] |
|------------|---------------------|---|
| PH□□ | Unlit | none : No temperature compensation |
| | CU 50 | CU 50 : Cu500 |

During this time, all outputs are in OFF status, and all LED indicators except the PWR indicator turns off.

After that, measurement starts, indicating the item selected in [Display selection (p.32)].

This status is called pH/Temperature Display Mode, or Cleansing Output Mode.

8.2 pH Input Group

To enter the pH Input group, follow the procedure below.

- ① F.n.c. 1 Press the  key in pH/Temperature Display Mode, or Cleansing Output Mode.
- ② 4EPH Press the  key.

The unit proceeds to the pH Input group, and 'pH 7 calibration standard' appears.

| Character | Setting Item, Function, Setting Range | Factory Default |
|----------------|---|------------------------------|
| TYPE JI 4□ | pH 7 calibration standard • Selects the pH 7 calibration value standard. • Not available if <i>MANU</i> (Manual) is selected in [pH calibration Auto/Manual]. • JI 4□ : JIS (Japanese Industrial Standards) U4□□ : US standard | JIS |
| 4EPH PH4□ | 2nd solution • Selects the 2nd solution for the automatic pH calibration from pH 2, pH 4, pH 9, pH 10 (JIS). [The 1st solution is fixed at pH 7 (JIS or US standard).] • Not available if <i>MANU</i> (Manual) is selected in [pH calibration Auto/Manual]. • PH2□ : pH 2 PH4□ : pH 4 PH9□ : pH 9 PH 10 : pH 10 (JIS: Japanese Industrial Standards) | pH 4 |
| dP 1□ □.000 | Decimal point place • Selects the decimal point place. • □.□□□ : No decimal point □.□□ : 1 digit after decimal point □.□□□ : 2 digits after decimal point | 2 digits after decimal point |

| Character | Setting Item, Function, Setting Range | Factory Default | | | | | | |
|--|--|--|--|--|--|---|---|--|
| A11 IF ----- | <p>A11 type</p> <ul style="list-style-type: none"> Selects an A11 type. <p>Note: If A11 type is changed, A11 value defaults to 0.00.</p> <ul style="list-style-type: none"> -----: No action <i>PH_L</i> : pH input low limit action (Fig. 8.2-1) <i>PH_H</i> : pH input high limit action (Fig. 8.2-1) <i>TEMP_L</i> : Temperature input low limit action (Fig. 8.2-1) <i>TEMP_H</i> : Temperature input high limit action (Fig. 8.2-1) <i>Error</i> : Error output [When the error type is "Error"(Table 8.2-1), the output is turned ON.] <i>FAIL</i> : Fail output [When the error type is "Fail" (Table 8.2-1), the output is turned ON.] <i>CLEO</i> : Cleansing output [10.6 Cleansing Output (P.46, 47)] <i>EPHA</i> : pH fluctuation alarm output [10.10 pH Fluctuation Alarm Output (P.48)] <i>PHHL</i> : pH input High/Low limits independent action (Fig. 8.2-2) <i>TEMPHL</i> : Temperature input High/Low limits independent action (Fig. 8.2-2) | No action | | | | | | |
| | <p>• A11 Action (Activated based on the indication value.)</p> <table border="1"> <thead> <tr> <th>pH input low limit action, Temperature input low limit action</th> <th>pH input high limit action, Temperature input high limit action</th> </tr> </thead> <tbody> <tr> <td> <p>If Medium Value is selected in [A11 hysteresis type]:</p> </td> <td> <p>If Medium Value is selected in [A11 hysteresis type]:</p> </td> </tr> <tr> <td> <p>If Reference Value is selected in [A11 hysteresis type]:</p> </td> <td> <p>If Reference Value is selected in [A11 hysteresis type]:</p> </td> </tr> </tbody> </table> <p>(Fig. 8.2-1)</p> <p>* Setting Example:</p> <p>If [A11 ON side (<i>A11 I U</i>)] is set to 0.00 or 0.0, A11 output can be turned ON at the value set in [A11 value (<i>A11 I</i>)].</p> <p>If [A11 OFF side (<i>A11 I L</i>)] is set to 0.00 or 0.0, A11 output can be turned OFF at the value set in [A11 value (<i>A11 I</i>)].</p> | pH input low limit action, Temperature input low limit action | pH input high limit action, Temperature input high limit action | <p>If Medium Value is selected in [A11 hysteresis type]:</p> | <p>If Medium Value is selected in [A11 hysteresis type]:</p> | <p>If Reference Value is selected in [A11 hysteresis type]:</p> | <p>If Reference Value is selected in [A11 hysteresis type]:</p> | |
| pH input low limit action, Temperature input low limit action | pH input high limit action, Temperature input high limit action | | | | | | | |
| <p>If Medium Value is selected in [A11 hysteresis type]:</p> | <p>If Medium Value is selected in [A11 hysteresis type]:</p> | | | | | | | |
| <p>If Reference Value is selected in [A11 hysteresis type]:</p> | <p>If Reference Value is selected in [A11 hysteresis type]:</p> | | | | | | | |
| | <table border="1"> <thead> <tr> <th>pH input High/Low limits independent action, Temperature input High/Low limits independent action</th> </tr> </thead> <tbody> <tr> <td> </td> </tr> </tbody> </table> <p>(Fig. 8.2-2)</p> | pH input High/Low limits independent action, Temperature input High/Low limits independent action | | | | | | |
| pH input High/Low limits independent action, Temperature input High/Low limits independent action | | | | | | | | |
| | | | | | | | | |

| Character | Setting Item, Function, Setting Range | Factory Default | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
|---------------|---|--|------------|----------------|-------------|-------|----------------------|--|-------|-----------------------------|---|-------|---------------------------|---|-------|-------------------------|---|-------|----------------------------|---|-------|-----------------------------|--|-------|-----------------------------|--|------|----------------------|--|------|------------------------------|--|
| | • Error output, Fail output (Table 8.2-1) <table border="1"> <thead> <tr> <th>Error Type</th> <th>Error Contents</th> <th>Description</th> </tr> </thead> <tbody> <tr> <td>Error</td> <td>Response Speed Error</td> <td>When calibrating, the response of the pH Combined Electrode Sensor is slow. When the difference between the input and each of the 1st and 2nd solutions are within pH ± 1.50, and input fluctuation is over pH ± 0.05 (in 10 seconds of assessment cycles) for 5 minutes, this is assumed to be an error. However, if input fluctuation is less than or equal to pH ± 0.05, this is assumed to be within the normal range.</td> </tr> <tr> <td>Error</td> <td>Electrode Sensitivity Error</td> <td>When calibrating, sensitivity of the pH Combined Electrode Sensor has deteriorated. The difference between 1st and 2nd standard solution value after calibration is less than or equal to pH 2.00.</td> </tr> <tr> <td>Error</td> <td>Asymmetry Potential Error</td> <td>When calibrating pH 7, the difference in electromotive force between the sensor-measured value and standard value exceeds the equivalent of pH ± 1.50.</td> </tr> <tr> <td>Error</td> <td>Standard Solution Error</td> <td>The specified standard solution has not been used. When pH ± 1.50 is exceeded for the 1st & 2nd solutions.</td> </tr> <tr> <td>Error</td> <td>Solution Temperature Error</td> <td>When temperature is higher than (and including) 55°C at pH 10 solution.</td> </tr> <tr> <td>Error</td> <td>Outside Temp. Compen. Range</td> <td>Measured temperature has exceeded 110.0°C.</td> </tr> <tr> <td>Error</td> <td>Outside Temp. Compen. Range</td> <td>Measured temperature is less than 0.0°C.</td> </tr> <tr> <td>Fail</td> <td>Temp. Sensor Burnout</td> <td>Temperature sensor lead wire is burnt out.</td> </tr> <tr> <td>Fail</td> <td>Temp. Sensor Short-circuited</td> <td>Temperature sensor lead wire is short-circuited.</td> </tr> </tbody> </table> <p>(Abbreviations: Temp.: Temperature, Compen.: Compensation)</p> | | Error Type | Error Contents | Description | Error | Response Speed Error | When calibrating, the response of the pH Combined Electrode Sensor is slow. When the difference between the input and each of the 1st and 2nd solutions are within pH ± 1.50 , and input fluctuation is over pH ± 0.05 (in 10 seconds of assessment cycles) for 5 minutes, this is assumed to be an error. However, if input fluctuation is less than or equal to pH ± 0.05 , this is assumed to be within the normal range. | Error | Electrode Sensitivity Error | When calibrating, sensitivity of the pH Combined Electrode Sensor has deteriorated. The difference between 1st and 2nd standard solution value after calibration is less than or equal to pH 2.00. | Error | Asymmetry Potential Error | When calibrating pH 7, the difference in electromotive force between the sensor-measured value and standard value exceeds the equivalent of pH ± 1.50 . | Error | Standard Solution Error | The specified standard solution has not been used. When pH ± 1.50 is exceeded for the 1st & 2nd solutions. | Error | Solution Temperature Error | When temperature is higher than (and including) 55°C at pH 10 solution. | Error | Outside Temp. Compen. Range | Measured temperature has exceeded 110.0°C. | Error | Outside Temp. Compen. Range | Measured temperature is less than 0.0°C. | Fail | Temp. Sensor Burnout | Temperature sensor lead wire is burnt out. | Fail | Temp. Sensor Short-circuited | Temperature sensor lead wire is short-circuited. |
| Error Type | Error Contents | Description | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Error | Response Speed Error | When calibrating, the response of the pH Combined Electrode Sensor is slow. When the difference between the input and each of the 1st and 2nd solutions are within pH ± 1.50 , and input fluctuation is over pH ± 0.05 (in 10 seconds of assessment cycles) for 5 minutes, this is assumed to be an error. However, if input fluctuation is less than or equal to pH ± 0.05 , this is assumed to be within the normal range. | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Error | Electrode Sensitivity Error | When calibrating, sensitivity of the pH Combined Electrode Sensor has deteriorated. The difference between 1st and 2nd standard solution value after calibration is less than or equal to pH 2.00. | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Error | Asymmetry Potential Error | When calibrating pH 7, the difference in electromotive force between the sensor-measured value and standard value exceeds the equivalent of pH ± 1.50 . | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Error | Standard Solution Error | The specified standard solution has not been used. When pH ± 1.50 is exceeded for the 1st & 2nd solutions. | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Error | Solution Temperature Error | When temperature is higher than (and including) 55°C at pH 10 solution. | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Error | Outside Temp. Compen. Range | Measured temperature has exceeded 110.0°C. | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Error | Outside Temp. Compen. Range | Measured temperature is less than 0.0°C. | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Fail | Temp. Sensor Burnout | Temperature sensor lead wire is burnt out. | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| Fail | Temp. Sensor Short-circuited | Temperature sensor lead wire is short-circuited. | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| A12F [---] | A12 type • Selects an A12 type. Note: If A12 type is changed, A12 value defaults to 0.00. • For the selection item and action, refer to [A11 type (pp. 21, 22)]. | No action | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| A21F [---] | A21 type • Selects an A21 type. Note: If A21 type is changed, A21 value defaults to 0.00. • For the selection item and action, refer to [A11 type (pp. 21, 22)]. | No action | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| A22F [---] | A22 type • Selects an A22 type. Note: If A22 type is changed, A22 value defaults to 0.00. • For the selection item and action, refer to [A11 type (pp. 21, 22)]. | No action | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| A11 [0.00] | A11 value • Selects an A11 value. • Not available if [---] (No action), <i>ErOF</i> (Error output), <i>FAIL</i> (Fail output), <i>CLC</i> (Cleansing output) is selected in [A11 type]. • Setting range: pH input: pH 0.00 to 14.00 (*) Temperature input: 0.0 to 100.0°C (*) (*) The placement of the decimal point does not follow the selection. It is fixed. | pH input: pH 0.00, Temperature input: 0.0°C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| A12 [0.00] | A12 value • Selects an A12 value. • For the indication condition and setting range, refer to [A11 type (pp. 21, 22)]. | pH input: pH 0.00, Temperature input: 0.0°C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| A21 [0.00] | A21 value • Selects an A21 value. • For the indication condition and setting range, refer to [A11 type (pp. 21, 22)]. | pH input: pH 0.00, Temperature input: 0.0°C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |
| A22 [0.00] | A22 value • Selects an A22 value. • For the indication condition and setting range, refer to [A11 type (pp. 21, 22)]. | pH input: pH 0.00, Temperature input: 0.0°C | | | | | | | | | | | | | | | | | | | | | | | | | | | | | | |

| Character | Setting Item, Function, Setting Range | Factory Default |
|---------------------------------------|--|---|
| A11d 4dl F | A11 hysteresis type <ul style="list-style-type: none"> • Selects A11 hysteresis type (Medium or Reference Value). • Not available if <input type="checkbox"/> <input type="checkbox"/> <input type="checkbox"/> <input type="checkbox"/> (No action), <i>ErOr</i> (Error output), <i>FRiL</i> (Fail output), <i>cLEG</i> (Cleansing output) is selected in [A11 type]. • <i>cdl F</i>: Medium Value Sets the same value for both ON and OFF sides in relation to A11 value. Only ON side needs to be set. <i>4dl F</i>: Reference Value Sets individual values for ON and OFF sides in relation to A11 value. Both ON and OFF sides need to be set individually. | Reference Value |
| A11U <input type="checkbox"/> 0.10 | A11 ON side <ul style="list-style-type: none"> • Sets the span of A11 ON side. If <i>cdl F</i> (Medium Value) is selected in [A11 hysteresis type], the span of ON/OFF side will be the same value. • Not available if <input type="checkbox"/> <input type="checkbox"/> <input type="checkbox"/> <input type="checkbox"/> (No action), <i>ErOr</i> (Error output), <i>FRiL</i> (Fail output), <i>cLEG</i> (Cleansing output) is selected in [A11 type]. • Setting range: pH input: pH 0.00 to 4.00 (*) Temperature input: 0.0 to 10.0°C (*) (*) The placement of the decimal point does not follow the selection. It is fixed. | pH input: pH 0.10, Temperature input: 1.0°C |
| A11L <input type="checkbox"/> 0.10 | A11 OFF side <ul style="list-style-type: none"> • Sets the span of A11 OFF side. • Not available if <i>cdl F</i> (Medium Value) is selected in [A11 hysteresis type]. • Not available if <input type="checkbox"/> <input type="checkbox"/> <input type="checkbox"/> <input type="checkbox"/> (No action), <i>ErOr</i> (Error output), <i>FRiL</i> (Fail output), <i>cLEG</i> (Cleansing output) is selected in [A11 type]. • Setting range: pH input: pH 0.00 to 4.00 (*) Temperature input: 0.0 to 10.0°C (*) (*) The placement of the decimal point does not follow the selection. It is fixed. | pH input: pH 0.10, Temperature input: 1.0°C |
| A12d 4dl F | A12 hysteresis type <ul style="list-style-type: none"> • Selects A12 hysteresis type (Medium or Reference Value). • For the indication condition and selection item, refer to [A11 hysteresis type]. | Reference Value |
| A12U <input type="checkbox"/> 0.10 | A12 ON side <ul style="list-style-type: none"> • Sets the span of A12 ON side. If <i>cdl F</i> (Medium Value) is selected in [A12 hysteresis type], the span of ON/OFF side will be the same value. • For the indication condition and setting range, refer to [A11 ON side]. | pH input: pH 0.10, Temperature input: 1.0°C |
| A12L <input type="checkbox"/> 0.10 | A12 OFF side <ul style="list-style-type: none"> • Sets the span of A12 OFF side. • For the indication condition and setting range, refer to [A11 OFF side]. | pH input: pH 0.10, Temperature input: 1.0°C |
| A21d 4dl F | A21 hysteresis type <ul style="list-style-type: none"> • Selects A21 hysteresis type (Medium or Reference Value). • For the indication condition and selection item, refer to [A11 hysteresis type]. | Reference Value |
| A21U <input type="checkbox"/> 0.10 | A21 ON side <ul style="list-style-type: none"> • Sets the span of A21 ON side. If <i>cdl F</i> (Medium Value) is selected in [A21 hysteresis type], the span of ON/OFF side will be the same value. • For the indication condition and setting range, refer to [A11 ON side]. | pH input: pH 0.10, Temperature input: 1.0°C |
| A21L <input type="checkbox"/> 0.10 | A21 OFF side <ul style="list-style-type: none"> • Sets the span of A21 OFF side. • For the indication condition and setting range, refer to [A11 OFF side]. | pH input: pH 0.10, Temperature input: 1.0°C |

| Character | Setting Item, Function, Setting Range | Factory Default |
|---------------|---|---|
| A22d 4d1 F | A22 hysteresis type • Selects A22 output hysteresis type (Medium or Reference Value). • For the indication condition and selection item, refer to [A11 hysteresis type (p.23)]. | Reference Value |
| A22U 00.10 | A22 ON side • Sets the span of A22 ON side. If 4d1 F (Medium Value) is selected in [A22 hysteresis type], the span of ON/OFF side will be the same value. • For the indication condition and setting range, refer to [A11 ON side (p.23)]. | pH input: pH 0.10, Temperature input: 1.0°C |
| A22L 00.10 | A22 OFF side • Sets the span of A22 OFF side. • For the indication condition and setting range, refer to [A11 OFF side (p.23)]. | pH input: pH 0.10, Temperature input: 1.0°C |
| A11a 0000 | A11 ON delay time • Sets A11 ON delay time. The A11 output does not turn ON (under the conditions of turning ON) until the time set in [A11 ON delay time] elapses. • Not available if 0000 (No action), Error (Error output), FAIL (Fail output), CLEAR (Cleansing output) is selected in [A11 type]. • Setting range: 0 to 9999 seconds | 0 seconds |
| A12a 0000 | A12 ON delay time • Sets A12 ON delay time. The A12 output does not turn ON (under the conditions of turning ON) until the time set in [A12 ON delay time] elapses. • For the indication condition and setting range, refer to [A11 ON delay time]. | 0 seconds |
| A21a 0000 | A21 ON delay time • Sets A21 ON delay time. The A21 output does not turn ON (under the conditions of turning ON) until the time set in [A21 ON delay time] elapses. • For the indication condition and setting range, refer to [A11 ON delay time]. | 0 seconds |
| A22a 0000 | A22 ON delay time • Sets A22 ON delay time. The A22 output does not turn ON (under the conditions of turning ON) until the time set in [A22 ON delay time] elapses. • For the indication condition and setting range, refer to [A11 ON delay time]. | 0 seconds |
| A11c 0000 | A11 OFF delay time • Sets A11 OFF delay time. The A11 output does not turn OFF (under the conditions of turning OFF) until the time set in [A11 OFF delay time] elapses. • Not available if 0000 (No action), Error (Error output), FAIL (Fail output), CLEAR (Cleansing output) is selected in [A11 type]. • Setting range: 0 to 9999 seconds | 0 seconds |
| A12c 0000 | A12 OFF delay time • Sets A12 OFF delay time. The A12 output does not turn OFF (under the conditions of turning OFF) until the time set in [A12 OFF delay time] elapses. • For the indication condition and setting range, refer to [A11 OFF delay time]. | 0 seconds |
| A21c 0000 | A21 OFF delay time • Sets A21 OFF delay time. The A21 output does not turn OFF (under the conditions of turning OFF) until the time set in [A21 OFF delay time] elapses. • For the indication condition and setting range, refer to [A11 OFF delay time]. | 0 seconds |

| Character | Setting Item, Function, Setting Range | Factory Default |
|--------------|--|---|
| A22c □□□□ | A22 OFF delay time • Sets A22 OFF delay time. The A22 output does not turn OFF (under the conditions of turning OFF) until the time set in [A22 OFF delay time] elapses. • For the indication condition and setting range, refer to [A11 OFF delay time (p.24)]. | 0 seconds |
| A11f □□□□ | A11 pH fluctuation alarm time • Sets time to assess A11 pH fluctuation alarm. Disabled when set to 0 (zero). • Available only when <i>EPHA</i> (pH fluctuation alarm output) is selected in [A11 type]. • Setting range: 0 to 72 hours | 0 hours |
| A12f □□□□ | A12 pH fluctuation alarm time • Sets time to assess A12 pH fluctuation alarm. • For the action, indication condition and setting range, refer to [A11 pH fluctuation alarm time]. | 0 hours |
| A21f □□□□ | A21 pH fluctuation alarm time • Sets time to assess A21 pH fluctuation alarm. • For the action, indication condition and setting range, refer to [A11 pH fluctuation alarm time]. | 0 hours |
| A22f □□□□ | A22 pH fluctuation alarm time • Sets time to assess A22 pH fluctuation alarm. • For the action, indication condition and setting range, refer to [A11 pH fluctuation alarm time]. | 0 hours |
| A114 □□□□ | A11 pH fluctuation alarm band • Sets the band to assess A11 pH fluctuation alarm. Disabled when set to pH 0.00. • Available only when <i>EPHA</i> (pH fluctuation alarm output) is selected in [A11 type]. • Setting range: pH 0.00 to 14.00 | pH 0.00 |
| A124 □□□□ | A12 pH fluctuation alarm band • Sets the band to assess A12 pH fluctuation alarm. • For the action, indication condition and setting range, refer to [A11 pH fluctuation alarm band]. | pH 0.00 |
| A214 □□□□ | A21 pH fluctuation alarm band • Sets the band to assess A21 pH fluctuation alarm. • For the action, indication condition and setting range, refer to [A11 pH fluctuation alarm band]. | pH 0.00 |
| A224 □□□□ | A22 pH fluctuation alarm band • Sets the band to assess A22 pH fluctuation alarm. • For the action, indication condition and setting range, refer to [A11 pH fluctuation alarm band]. | pH 0.00 |
| A11n □□□□ | A11 High/Low limits independent lower side band • Sets the lower side band of A11 High/Low limits independent action. Disabled when set to pH 0.00 or 0.0°C. • Available when <i>PHHL</i> (pH input High/Low limits independent action) or <i>TnHL</i> (Temperature input High/Low limits independent action) is selected in [A11 type]. • Setting range: pH input: pH 0.00 to 14.00 (*) Temperature input: 0.0 to 100.0°C(*) (*) The placement of the decimal point does not follow the selection. It is fixed. | pH input: pH 0.00, Temperature input: 0.0°C |
| A12n □□□□ | A12 High/Low limits independent lower side band • Sets the lower side band of A12 High/Low limits independent action. • For the action, indication condition and setting range, refer to [A11 High/Low limits independent lower side band]. | pH input: pH 0.00, Temperature input: 0.0°C |

| Character | Setting Item, Function, Setting Range | Factory Default |
|------------------------|---|---|
| <i>A2 Ln</i> □.000 | A21 High/Low limits independent lower side band <ul style="list-style-type: none"> Sets the lower side band of A21 High/Low limits independent action. For the action, indication condition and setting range, refer to [A11 High/Low limits independent lower side band (p.25)]. | pH input: pH 0.00, Temperature input: 0.0°C |
| <i>A22 Ln</i> □.000 | A22 High/Low limits independent lower side band <ul style="list-style-type: none"> Sets the lower side band of A22 High/Low limits independent action. For the action, indication condition and setting range, refer to [A11 High/Low limits independent lower side band (p.25)]. | pH input: pH 0.00, Temperature input: 0.0°C |
| <i>A11 P</i> □.000 | A11 High/Low limits independent upper side band <ul style="list-style-type: none"> Sets the upper side band of A11 High/Low limits independent action. Disabled when set to pH 0.00 or 0.0°C. Available when <i>P_{HH}L</i> (pH input High/Low limits independent action) or <i>T_{NH}L</i> (Temperature input High/Low limits independent action) is selected in [A11 type]. Setting range: pH input: pH 0.00 to 14.00 (*) Temperature input: 0.0 to 100.0°C (*) (*) The placement of the decimal point does not follow the selection. It is fixed. | pH input: pH 0.00, Temperature input: 0.0°C |
| <i>A12 P</i> □.000 | A12 High/Low limits independent upper side band <ul style="list-style-type: none"> Sets the upper side band of A12 High/Low limits independent action. For the action, indication condition and setting range, refer to [A11 High/Low limits independent upper side band]. | pH input: pH 0.00, Temperature input: 0.0°C |
| <i>A21 P</i> □.000 | A21 High/Low limits independent upper side band <ul style="list-style-type: none"> Sets the upper side band of A21 High/Low limits independent action. For the action, indication condition and setting range, refer to [A11 High/Low limits independent upper side band]. | pH input: pH 0.00, Temperature input: 0.0°C |
| <i>A22 P</i> □.000 | A22 High/Low limits independent upper side band <ul style="list-style-type: none"> Sets the upper side band of A22 High/Low limits independent action. For the action, indication condition and setting range, refer to [A11 High/Low limits independent upper side band]. | pH input: pH 0.00, Temperature input: 0.0°C |
| <i>A11 H</i> □.0.10 | A11 hysteresis <ul style="list-style-type: none"> Sets hysteresis of A11 High/Low limits independent action. Available when <i>P_{HH}L</i> (pH input High/Low limits independent action) or <i>T_{NH}L</i> (Temperature input High/Low limits independent action) is selected in [A11 type]. Setting range: pH input: pH 0.01 to pH 4.00 (*) Temperature input: 0.1 to 10.0°C (*) (*) The placement of the decimal point does not follow the selection. It is fixed. | pH input: pH 0.10, Temperature input: 1.0°C |
| <i>A12 H</i> □.0.10 | A12 hysteresis <ul style="list-style-type: none"> Sets hysteresis of A12 High/Low limits independent action. For the indication condition and setting range, refer to [A11 hysteresis]. | pH input: pH 0.10, Temperature input: 1.0°C |
| <i>A21 H</i> □.0.10 | A21 hysteresis <ul style="list-style-type: none"> Sets hysteresis of A21 High/Low limits independent action. For the indication condition and setting range, refer to [A11 hysteresis]. | pH input: pH 0.10, Temperature input: 1.0°C |
| <i>A22 H</i> □.0.10 | A22 hysteresis <ul style="list-style-type: none"> Sets hysteresis of A22 High/Low limits independent action. For the indication condition and setting range, refer to [A11 hysteresis]. | pH input: pH 0.10, Temperature input: 1.0°C |

| Character | Setting Item, Function, Setting Range | Factory Default |
|----------------------|--|-----------------|
| <i>IErr</i> OFF | A□□ output when input errors occur <ul style="list-style-type: none"> If input errors occur, such as pH Combined Electrode Sensor is burnt out or short-circuited, A□□ output Enabled/Disabled can be selected. If “Enabled” is selected, A□□ output and A□□ output status will be maintained when input errors occur. If “Disabled” is selected, A□□ output and A□□ output status will be turned OFF when input errors occur. Available when <i>PH_L</i> (pH input low limit action), <i>PH_H</i> (pH input high limit action), <i>TnPL</i> (Temperature input low limit action), or <i>TnPH</i> (Temperature input high limit action) is selected in [A□□ type]. Selection item: ON : Enabled OFF : Disabled | Disabled |
| <i>FILT</i> □□.□□ | pH input filter time constant <ul style="list-style-type: none"> Sets pH input filter time constant. If the value is set too large, it affects A□□ output due to the delay of response. Setting range: 0.0 to 60.0 seconds | 0.0 seconds |
| <i>pHc</i> □□.□□ | pH input sensor correction <ul style="list-style-type: none"> Sets pH input sensor correction value. This corrects the measured value from the pH Combined Electrode Sensor. When a sensor cannot be set at the exact location where measurement is desired, pH value measured by the sensor may deviate from the pH in the measured location. In this case, desired pH can be obtained by adding a sensor correction value. However, it is effective within the measurement range regardless of the sensor correction value. pH value after sensor correction = Current pH value + (Sensor correction value) Setting range: pH -1.40 to 1.40 (*) (*) The placement of the decimal point does not follow the selection. It is fixed. | 0.00 |
| <i>dFct</i> □□.□□ | pH inputs for moving average <ul style="list-style-type: none"> Sets the number of pH inputs used to obtain a moving average. An average pH input value is calculated using the selected number of pH inputs. The pH input value is replaced every input sampling period. However, the pH input moving average function is disabled in pH calibration mode. Setting range: 1 to 120 | 20 |

8.3 Temperature Input Group

To enter the Temperature Input group, follow the procedure below.

- ① *F.n.c.2* Press the  key twice in pH/Temperature Display Mode, or Cleansing Output Mode.
- ② *4E n4* Press the  key.

The unit enters the Temperature Input group, and 'Electrode RTD' appears.

| Character | Setting Item, Function, Setting Range | Factory Default |
|------------------------------|---|-----------------------------------|
| <i>4E n4</i> <i>Pf 10</i> | Electrode RTD <ul style="list-style-type: none"> • Selects RTD type of the electrode. • Depending on the input specification, the following items can be selected. Pt spec <i>nonE</i> : No temperature compensation <i>Pf 10</i> : Pt1000 <i>Pf 100</i> : Pt100 Cu spec <i>nonE</i> : No temperature compensation <i>cU500</i> : Cu500 | Pt spec: Pt1000 Cu spec: Cu500 |
| <i>4T nd</i> <i>025.0</i> | Reference temperature <ul style="list-style-type: none"> • Sets the reference temperature for temperature compensation. • If <i>nonE</i> (No temperature compensation) is selected in [Electrode RTD], the temperature set in [Reference temperature] will be indicated on the Temperature Display. • Setting range: 5.0 to 95.0°C (*) (*) The placement of the decimal point does not follow the selection. It is fixed. | 25.0°C |
| <i>dP20</i> <i>0000</i> | Decimal point place <ul style="list-style-type: none"> • Selects decimal point place. • <i>0000</i>: No decimal point • <i>0000</i>: 1 digit after decimal point | 1 digit after decimal point |
| <i>conE</i> <i>Pf 03</i> | Pt100 input wire type <ul style="list-style-type: none"> • Selects the input wire type when Pt100 is selected in [Electrode RTD]. • Available only when <i>Pf 100</i> (Pt100) is selected in [Electrode RTD]. • <i>Pf 02</i>: 2-wire type • <i>Pf 03</i>: 3-wire type | 3-wire type |
| <i>cAbL</i> <i>0000</i> | Cable length correction <ul style="list-style-type: none"> • Sets the cable length correction value. • Available when <i>Pf 100</i> (Pt100) is selected in [Electrode RTD]. • Available when <i>Pf 02</i> (2-wire Type) is selected in [Pt100 input wire type]. • Setting Range: 0.0 to 100.0 m | 0.0 m |
| <i>c4Ec</i> <i>00.30</i> | Cable cross-section area <ul style="list-style-type: none"> • Sets the cable cross-section area. • Available when <i>Pf 100</i> (Pt100) is selected in [Electrode RTD]. • Available when <i>Pf 02</i> (2-wire Type) is selected in [Pt100 input wire type]. • Setting Range: 0.10 to 2.00 mm² | 0.30 mm ² |
| <i>dF cT</i> <i>0020</i> | Temperature inputs for moving average <ul style="list-style-type: none"> • Sets the number of temperature inputs used to obtain a moving average. • An average temperature input value is calculated using the selected number of temperature inputs. The temperature input value is replaced every input sampling period. However, the temperature input moving average function is disabled in temperature calibration mode. • Setting range: 1 to 120 | 20 |

8.4 Basic Function Group

To enter the Basic Function group, follow the procedure below.

- ① *Off* Press the  key 3 times in pH/Temperature Display Mode, or Cleansing Output Mode.
- ② *Lock* Press the  key.

The unit enters the Basic Function group, and the 'Set value lock' appears.

| Character | Setting Item, Function, Setting Range | Factory Default |
|--|--|-----------------|
| <i>Lock</i> - - - - | Set value lock <ul style="list-style-type: none"> • Locks the set values to prevent setting errors. •  (Unlock): All set values can be changed. • <i>Loc 1</i> (Lock 1): None of the set values can be changed. • <i>Loc 2</i> (Lock 2): Only A11, A12, A21, A22 values can be changed. • <i>Loc 3</i> (Lock 3): All set values – except Electrode RTD, Temperature calibration value, pH calibration value, pH calibration Auto/Manual, Transmission output 1 Zero adjustment value, Transmission output 1 Span adjustment value, Transmission output 2 Zero adjustment value, Transmission output 2 Span adjustment value – can be temporarily changed. However, they revert to their previous value after the power is turned off because they are not saved in the non-volatile IC memory. <p>Do not change setting items (A11, A12, A21, A22 types). If they are changed, they will affect other setting items.</p> <p>Be sure to select Lock 3 when changing the set value frequently via software communication. (If a value set via software communication is the same as the value before the setting, the value will not be written in non-volatile IC memory.)</p> | Unlock |
| <i>cn4L</i> <i>nonL</i> | Communication protocol <ul style="list-style-type: none"> • Selects communication protocol. • <i>nonL</i> : Shinko protocol • <i>nodA</i> : MODBUS ASCII mode • <i>nodr</i> : MODBUS RTU mode | Shinko protocol |
| <i>cnno</i>  | Instrument number <ul style="list-style-type: none"> • Sets the instrument number. (The instrument numbers should be set one by one when multiple instruments are connected.) • Setting range: 0 to 95 | 0 |
| <i>cn4P</i>  | Communication speed <ul style="list-style-type: none"> • Selects a communication speed equal to that of the host computer. •  : 9600 bps •  : 19200 bps •  : 38400 bps | 9600 bps |
| <i>cnFF</i> <i>7EEn</i> | Data bit/Parity <ul style="list-style-type: none"> • Selects data bit and parity. • <i>8non</i> : 8 bits/No parity • <i>7non</i> : 7 bits/No parity • <i>8EEn</i> : 8 bits/Even • <i>7EEn</i> : 7 bits/Even • <i>8odd</i> : 8 bits/Odd • <i>7odd</i> : 7 bits/Odd | 7 bits/Even |
| <i>cn4f</i>  | Stop bit <ul style="list-style-type: none"> • Selects the stop bit. •  : 1 bit •  : 2 bits | 1 bit |

| Character | Setting Item, Function, Setting Range | Factory Default |
|--------------------|--|--------------------------|
| T r o 1 P H □ □ | Transmission output 1 type <ul style="list-style-type: none"> • Selects Transmission output 1 type. If <i>n o n E</i> (No Temperature Compensation) is selected in [Electrode RTD (p.28)], and if <i>T E M P</i> (Temperature transmission) is selected in [Transmission output 1 type], the value set in [Reference temperature (p.28)] will be output. • Available only when Transmission output 1 (TA option) or Transmission output 2 (TA2 option) is ordered. • <i>P H □ □</i> : pH transmission <i>T E M P</i> : Temperature transmission | pH transmission |
| T r H 1 1400 | Transmission output 1 high limit <ul style="list-style-type: none"> • Sets the Transmission output 1 high limit value. (This value corresponds to 20 mA DC output.) If Transmission output 1 high limit and low limit are set to the same value, Transmission output 1 will be fixed at 4 mA DC. • Available when Transmission output 1 (TA option) or Transmission output 2 (TA2 option) is ordered. • Setting range: When <i>P H □ □</i> (pH Transmission) is selected in [Transmission output 1 type]: Transmission output 1 low limit to pH 14.00 (*) When <i>T E M P</i> (Temperature Transmission) is selected in [Transmission output 1 type]: Transmission output 1 low limit to 100.0°C (*) (*) The placement of the decimal point does not follow the selection. It is fixed. | pH 14.00 |
| T r L 1 □ □ □ □ | Transmission output 1 low limit <ul style="list-style-type: none"> • Sets the Transmission output 1 low limit value. (This value corresponds to 4 mA DC output.) If Transmission output 1 high limit and low limit are set to the same value, Transmission output 1 will be fixed at 4 mA DC. • Available when Transmission output 1 (TA option) or Transmission output 2 (TA2 option) is ordered. • Setting range: When <i>P H □ □</i> (pH Transmission) is selected in [Transmission output 1 type]: pH 0.00 to Transmission output 1 high limit (*) When <i>T E M P</i> (Temperature Transmission) is selected in [Transmission output 1 type]: 0.0°C to Transmission output 1 high limit (*) (*) The placement of the decimal point does not follow the selection. It is fixed. | pH 0.00 |
| T r o 2 T E M P | Transmission output 2 type <ul style="list-style-type: none"> • Selects Transmission output 2 type. If <i>n o n E</i> (No Temperature Compensation) is selected in [Electrode RTD (p.28)], and if <i>T E M P</i> (Temperature transmission) is selected in [Transmission output 2 type], the value set in [Reference temperature (p.28)] will be output. • Available only when Transmission output 2 (TA2 option) is ordered. • <i>P H □ □</i> : pH transmission <i>T E M P</i> : Temperature transmission | Temperature transmission |
| T r H 2 1000 | Transmission output 2 high limit <ul style="list-style-type: none"> • Sets the Transmission output 2 high limit value. (This value corresponds to 20 mA DC output.) If Transmission output 2 high limit and low limit are set to the same value, Transmission output 2 will be fixed at 4 mA DC. • Available only when Transmission output 2 (TA2 option) is ordered. • Setting range: When <i>P H □ □</i> (pH Transmission) is selected in [Transmission output 2 type]: Transmission output 2 low limit to pH 14.00 (*) When <i>T E M P</i> (Temperature Transmission) is selected in [Transmission output 2 type]: Transmission output 2 low limit to 100.0°C (*) (*) The placement of the decimal point does not follow the selection. It is fixed. | 100.0°C |

| Character | Setting Item, Function, Setting Range | Factory Default |
|----------------------------|--|---|
| <i>rFL2</i> □□.□□ | Transmission output 2 low limit <ul style="list-style-type: none"> Sets the Transmission output 2 low limit value. (This value corresponds to 4 mA DC output.) If Transmission output 2 high limit and low limit are set to the same value, Transmission output 2 will be fixed at 4 mA DC. Available only when Transmission output 2 (TA2 option) is ordered. Setting range: When <i>PH</i>□□ (pH Transmission) is selected in [Transmission output 2 type]: pH 0.00 to Transmission output 2 high limit (*) When <i>TEMP</i> (Temperature Transmission) is selected in [Transmission output 2 type]: 0.0°C to Transmission output 2 high limit (*) (*) The placement of the decimal point does not follow the selection. It is fixed. | 0.0°C |
| <i>rFc1</i> <i>bEFH</i> | Transmission output 1 status when calibrating <ul style="list-style-type: none"> Selects Transmission output 1 output status when calibrating pH. Available when Transmission output 1 (TA option) or Transmission output 2 (TA2 option) is ordered. Selection item: <i>bEFH</i>: Last value HOLD (Retains the last value before pH calibration, and outputs it.) <i>SETH</i>: Set value HOLD (Outputs the value set in [Transmission output 1 value HOLD when calibrating].) <i>PH</i>□: Measured value (Outputs the measured value when calibrating pH.) | Last value HOLD |
| <i>rF41</i> □□.□□ | Transmission output 1 value HOLD when calibrating <ul style="list-style-type: none"> Sets Transmission output 1 value HOLD. Available only when <i>SETH</i> (Set value HOLD) is selected in [Transmission output 1 status when calibrating]. Setting range: When <i>PH</i>□□ (pH Transmission) is selected in [Transmission output 1 type]: pH 0.00 to 14.00 (*) When <i>TEMP</i> (Temperature Transmission) is selected in [Transmission output 1 type]: 0.0 to 100.0°C (*) (*) The placement of the decimal point does not follow the selection. It is fixed. | pH transmission: pH 0.00 Temperature transmission: 0.0°C |
| <i>rFc2</i> <i>bEFH</i> | Transmission output 2 status when calibrating <ul style="list-style-type: none"> Selects Transmission output 2 output status when calibrating pH. Available only when Transmission output 2 (TA2 option) is ordered. Selection range <i>bEFH</i>: Last value HOLD (Retains the last value before pH calibration, and outputs it.) <i>SETH</i>: Set value HOLD (Outputs the value set in [Transmission output 2 value HOLD when calibrating].) <i>PH</i>□: Measured value (Outputs the measured value when calibrating pH.) | Last value HOLD |
| <i>rF42</i> □□.□□ | Transmission output 2 value HOLD when calibrating <ul style="list-style-type: none"> Sets Transmission output 2 value HOLD. Available only when <i>SETH</i> (Set value HOLD) is selected in [Transmission output 2 status when calibrating]. Setting range: When <i>PH</i>□□ (pH Transmission) is selected in [Transmission output 2 type]: pH 0.00 to 14.00 (*) When <i>TEMP</i> (Temperature Transmission) is selected in [Transmission output 2 type]: 0.0 to 100.0°C (*) (*) The placement of the decimal point does not follow the selection. It is fixed. | pH transmission: pH 0.00 Temperature transmission: 0.0°C |
| <i>rU4F</i> <i>rUFa</i> | pH calibration Auto/Manual <ul style="list-style-type: none"> Selects either automatic or manual pH calibration. <i>rUFa</i> : Automatic <i>rANU</i> : Manual | Automatic |
| <i>LIGF</i> □□□□ | Auto-light function <ul style="list-style-type: none"> Selects Auto-light Enabled/Disabled. □□□□ : Disabled <i>U4E</i>□ : Enabled | Disabled |

| Character | Setting Item, Function, Setting Range | Factory Default | | | | | | | | | | | | | | | |
|---------------|--|---------------------|------------|---------------------|------|----|-------------|-----|----|---------------|------|---------------|-------------|------|---------------|---------------|----------------|
| d1 4P ALL□ | Display selection <ul style="list-style-type: none"> • Selects items to be indicated on the pH Display and Temperature Display. • Selection: (Table 8.4-1) <table border="1"> <thead> <tr> <th></th> <th>pH Display</th> <th>Temperature Display</th> </tr> </thead> <tbody> <tr> <td>ALL□</td> <td>pH</td> <td>Temperature</td> </tr> <tr> <td>PH□</td> <td>pH</td> <td>No indication</td> </tr> <tr> <td>TEMP</td> <td>No indication</td> <td>Temperature</td> </tr> <tr> <td>none</td> <td>No indication</td> <td>No indication</td> </tr> </tbody> </table> | | pH Display | Temperature Display | ALL□ | pH | Temperature | PH□ | pH | No indication | TEMP | No indication | Temperature | none | No indication | No indication | pH/Temperature |
| | pH Display | Temperature Display | | | | | | | | | | | | | | | |
| ALL□ | pH | Temperature | | | | | | | | | | | | | | | |
| PH□ | pH | No indication | | | | | | | | | | | | | | | |
| TEMP | No indication | Temperature | | | | | | | | | | | | | | | |
| none | No indication | No indication | | | | | | | | | | | | | | | |
| TIME 0000 | Indication time <ul style="list-style-type: none"> • Sets the indication time of the displays from no key operation until displays turn off. Displays remain lit when set to 00.00. Displays light up when any key is pressed while in unlit status. • Not available if none (No indication) is selected in [Display selection]. • Setting range: 00.00 (Remains lit) 00.01 to 60.00 (Minutes.Seconds) | 00.00 | | | | | | | | | | | | | | | |
| oFdP oFF□ | Temperature Display when no temperature compensation <ul style="list-style-type: none"> • If none (No temperature compensation) is selected in [Electrode RTD], the reference temperature set in [Reference temperature] can be indicated on the Temperature Display. • Available only when none (No temperature compensation) is selected in [Electrode RTD (p.28)]. • 4Fd□ : Reference temperature oFF□ : Unlit | Unlit | | | | | | | | | | | | | | | |
| A1oF A1□ | A1 output allocation <ul style="list-style-type: none"> • Selects A1 output allocation. For A1 output, A11 type, A12 type, A21 type and/or A22 type can be allocated. Output is OR output. However, if cLE□ (Cleansing output) is selected in any one of [A11, A12, A21, A22 type (pp. 21 22)], the Cleansing output will be given priority. • Not Available if Transmission output 2 (TA2 option) is ordered. • A1□ : A11 type A12□ : A12 type A21□ : A21 type A22□ : A22 type A1A1 : A11, A12 types A2A1 : A21, A22 types A1A2 : A11, A21 types A2A2 : A12, A22 types ALL□ : A11, A12, A21, A22 types | A11 type | | | | | | | | | | | | | | | |
| A2oF A2□ | A2 output allocation <ul style="list-style-type: none"> • Selects A2 output allocation. For A2 output, A11 type, A12 type, A21 type and/or A22 type can be allocated. Output is OR output. However, if cLE□ (Cleansing output) is selected in any one of [A11, A12, A21, A22 type (pp.21 22)], the Cleansing output will be given priority. • Not available if Transmission output 1 (TA option) or Transmission output 2 (TA2 option) is ordered. • For the selection item, refer to [A1 output allocation]. | A21 type | | | | | | | | | | | | | | | |

| Character | Setting Item, Function, Setting Range | Factory Default |
|--------------|--|-----------------|
| 00n1 0000 | Output ON time when A1 output ON <ul style="list-style-type: none"> Sets the Output ON time when A1 output is ON. If Output ON time and OFF time are set, A1 output can be turned ON/OFF in a configured cycle when A1 output is ON. (Fig. 8.4-1) Not available if Transmission output 2 (TA2 option) is ordered. Setting range: 0 to 9999 seconds <p style="text-align: center;">Timing chart (Output ON time and OFF time when A1 output is ON)</p> <p style="text-align: center;">(Fig. 8.4-1)</p> | 0 seconds |
| 00F1 0000 | Output OFF time when A1 output ON <ul style="list-style-type: none"> Sets Output OFF time when A1 output is ON. If Output ON time and OFF time are set, A1 output can be turned ON/OFF in a configured cycle when A1 output is ON. (Fig. 8.4-1) Not available if Transmission output 2 (TA2 option) is ordered. Setting range: 0 to 9999 seconds | 0 seconds |
| 00n2 0000 | Output ON time when A2 output ON <ul style="list-style-type: none"> Sets Output ON time when A2 output is ON. If Output ON time and OFF time are set, A2 output can be turned ON/OFF in a configured cycle when A2 output is ON. (Fig. 8.4-1) Not available if Transmission output 1 (TA option) or Transmission output 2 (TA2 option) is ordered. Setting range: 0 to 9999 seconds | 0 seconds |
| 00F2 0000 | Output OFF time when A2 output ON <ul style="list-style-type: none"> Sets Output OFF time when A2 output is ON. If Output ON time and OFF time are set, A2 output can be turned ON/OFF in a configured cycle when A2 output is ON. (Fig. 8.4-1) Not available if Transmission output 1 (TA option) or Transmission output 2 (TA2 option) is ordered. Setting range: 0 to 9999 seconds | 0 seconds |

| Character | Setting Item, Function, Setting Range | Factory Default |
|--------------|---|-----------------|
| A1P□ □□□□ | A1 pH input error alarm A□□ type <ul style="list-style-type: none"> • Selects A□□ type in order to assess A1 pH input error alarm. • Not available if Transmission output 2 (TA2 option) is ordered. • Selection item <ul style="list-style-type: none"> □□□□ : No action A11□ : A11 type A12□ : A12 type A21□ : A21 type A22□ : A22 type | No action |
| A2P□ □□□□ | A2 pH input error alarm A□□ type <ul style="list-style-type: none"> • Selects A□□ type in order to assess A2 pH input error alarm. • Not available if Transmission output 1 (TA option) or Transmission output 2 (TA2 option) is ordered. • For the selection item, refer to [A1 pH input error alarm A□□ type]. | No action |
| A1P□ □□□□ | A1 pH input error alarm band when A□□ output ON <ul style="list-style-type: none"> • Sets the band to assess A1 pH input error alarm when A□□ output (selected in [A1 pH input error alarm A□□ type]) is ON. Refer to Section '10.3 pH Input Error Alarm' on p.46. • Not available if Transmission output 2 (TA2 option) is ordered. • Setting range: pH 0.00 to 14.00 When set to 0.00, pH input error alarm is disabled. | pH 0.00 |
| A1P□ □□□□ | A1 pH input error alarm time when A□□ output ON <ul style="list-style-type: none"> • Sets time to assess A1 pH input error alarm when A□□ output (selected in [A1 pH input error alarm A□□ type]) is ON. Refer to Section '10.3 pH Input Error Alarm' on p.46. • Not available if Transmission output 2 (TA2 option) is ordered. • Setting range: 0 to 9999 seconds or minutes (Time unit follows the selection in [pH input error alarm time unit].) When set to 0, pH input error alarm is disabled. | 0 seconds |
| A1P□ □□□□ | A1 pH input error alarm band when A□□ output OFF <ul style="list-style-type: none"> • Sets the band to assess A1 pH input error alarm when A□□ output (selected in A1 pH input error alarm A□□ type) is OFF. Refer to Section '10.3 pH Input Error Alarm' on p.46. • Not available if Transmission output 2 (TA2 option) is ordered. • Setting range: pH 0.00 to 14.00 When set to 0.00, pH input error alarm is disabled. | pH 0.00 |

| Character | Setting Item, Function, Setting Range | Factory Default |
|--------------------------|--|-----------------|
| A1 _{EF} □□□□ | A1 pH input error alarm time when A□□ output OFF <ul style="list-style-type: none"> Sets time to assess A1 pH input error alarm when A□□ output (selected in [A1 pH input error alarm A□□ type]) is OFF. Refer to Section '10.3 pH Input Error Alarm' on p.46. Not available if Transmission output 2 (TA2 option) is ordered. Setting range: 0 to 9999 seconds or minutes (Time unit follows the selection in [pH input error alarm time unit].) When set to 0, pH input error alarm is disabled. | 0 seconds |
| A2P _b □□□□ | A2 pH input error alarm band when A□□ output ON <ul style="list-style-type: none"> Sets the band to assess A2 pH input error alarm when A□□ output (selected in [A2 pH input error alarm A□□ type]) is ON. Refer to Section '10.3 pH Input Error Alarm' on p.46. Not available if Transmission output 1 (TA option) or Transmission output 2 (TA2 option) is ordered. Setting range: pH 0.00 to 14.00 When set to 0.00, pH input error alarm is disabled. | pH 0.00 |
| A2 _{oF} □□□□ | A2 pH input error alarm time when A□□ output ON <ul style="list-style-type: none"> Sets time to assess A2 pH input error alarm when A□□ output (selected in [A2 pH input error alarm A□□ type]) is ON. Refer to Section '10.3 pH Input Error Alarm' on p.46. Not available if Transmission output 1 (TA option) or Transmission output 2 (TA2 option) is ordered. Setting range: 0 to 9999 seconds or minutes (Time unit follows the selection in [pH input error alarm time unit].) When set to 0, pH input error alarm is disabled. | 0 seconds |
| A2P _c □□□□ | A2 pH input error alarm band when A□□ output OFF <ul style="list-style-type: none"> Sets the band to assess A2 pH input error alarm when A□□ output (selected in [A2 pH input error alarm A□□ type]) is OFF. Refer to Section '10.3 pH Input Error Alarm' on p.46. Not available if Transmission output 1 (TA option) or Transmission output 2 (TA2 option) is ordered. Setting range: pH 0.00 to 14.00 When set to 0.00, pH input error alarm is disabled. | pH 0.00 |
| A2 _{cF} □□□□ | A2 pH input error alarm time when A□□ output OFF <ul style="list-style-type: none"> Sets time to assess A2 pH input error alarm when A□□ output (selected in [A2 pH input error alarm A□□ type]) is OFF. Refer to Section '10.3 pH Input Error Alarm' on p.46. Not available if Transmission output 1 (TA option) or Transmission output 2 (TA2 option) is ordered. Setting range: 0 to 9999 seconds or minutes (Time unit follows the selection in [pH input error alarm time unit].) When set to 0, pH input error alarm is disabled. | 0 seconds |

| Character | Setting Item, Function, Setting Range | Factory Default |
|-----------------------------|---|---|
| \bar{n}_4 $\text{4E}c$ | pH input error alarm time unit • Selects the time unit of pH input error alarm. • Selection item $\text{4E}c$: Second(s) $\bar{n}1\ n$: Minute(s) | Second(s) |
| $c c n f$ 0000 | Number of cleansing cycles • Sets the number of cleansing outputs. (Fig. 8.4-2) (p.37) • Available for this setting item and all subsequent items if $c L E c$ (Cleansing output) is selected in any one of [A11, A12, A21, A22 type (pp.21, 22)]. • Setting range: 0 to 10 (0: Continuous cleansing) | 0 (Continuous cleansing) |
| $c c y c$ 0360 | Cleansing interval • Sets an interval between cleansings. (Fig. 8.4-2) (p.37) • Setting range: 60 to 3000 minutes | 360 minutes |
| $c f 1 \bar{n}$ 0600 | Cleansing time • Sets the cleansing output time during the cleansing output interval. (Fig. 8.4-2) (p.37) • Setting range: 1 to 1800 seconds | 600 seconds |
| $c r E c$ 0600 | Restore time after cleansing • Sets the time to restore instruments to normal operation after cleansing output. (Fig. 8.4-2) (p.37) • Setting range: 1 to 1800 seconds | 600 seconds |
| $c c y 1$ $b E F H$ | Transmission output 1 status when cleansing • Selects Transmission output 1 output status when cleansing action is performing. • Available when Transmission output 1 (TA option) or Transmission output 2 (TA2 option) is ordered. • $b E F H$: Last value HOLD (Retains the last value before cleansing action, and outputs it.) $\text{4E}fH$: Set value HOLD (Outputs the value set in [Transmission output 1 value HOLD when cleansing].) $P y H$: Measured value (Outputs the measured value when cleansing action is performing.) | Last value HOLD |
| $c c E 1$ 0000 | Transmission output 1 value HOLD when cleansing • Sets the Transmission output 1 value HOLD. • Available only when $\text{4E}fH$ (Set value HOLD) is selected in [Transmission output 1 status when cleansing]. • Setting range: When $P y$ (pH Transmission) is selected in [Transmission output 1 type]: pH 0.00 to 14.00 (*) When $f E \bar{n} P$ (Temperature Transmission) is selected in [Transmission output 1 type]: 0.0 to 100.0°C (*) (*) The placement of the decimal point does not follow the selection. It is fixed. | pH transmission: pH 0.00 Temperature transmission: 0.0°C |
| $c c y 2$ $b E F H$ | Transmission output 2 status when cleansing • Selects Transmission output 2 output status when cleansing action is performing. • Available only when Transmission output 2 (TA2 option) is ordered. • $b E F H$: Last value HOLD (Retains the last value before cleansing action, and outputs it.) $\text{4E}fH$: Set value HOLD (Outputs the value set in [Transmission output 2 value HOLD when cleaning].) $P y H$: Measured value (Outputs the measured value when cleansing action is performing.) | Last value HOLD |
| $c c E 2$ 0000 | Transmission output 2 value HOLD when cleansing • Sets the Transmission output 2 value HOLD. • Available only when $\text{4E}fH$ (Set value HOLD) is selected in [Transmission output 2 status when cleansing]. • Setting range: When $P y$ (pH Transmission) is selected in [Transmission output 2 type]: pH 0.00 to 14.00 (*) When $f E \bar{n} P$ (Temperature Transmission) is selected in [Transmission output 2 type]: 0.0 to 100.0°C (*) (*) The placement of the decimal point does not follow the selection. It is fixed. | pH transmission: pH 0.00 Temperature transmission: 0.0°C |

• **pH Input Error Alarm**

pH input error alarm is used for detecting actuator trouble.


Even if pH input error alarm time has elapsed – if the change in pH input is smaller than the pH input error alarm band – the instrument assumes that actuator trouble has occurred, and sets Status flag 2 (A1, A2 pH input error alarm output flag bit).

In Serial communication, status can be read by reading Status flag 2 (A1, A2 pH input error alarm output flag bit).

pH input error alarm is enabled only when PH_L (pH input low limit action) PH_H (pH input high limit action) is selected in [A11, A12, A21, A22 type (p.21, 22)].

pH input error alarm is disabled during pH calibration.

• **Cleansing Output Action**

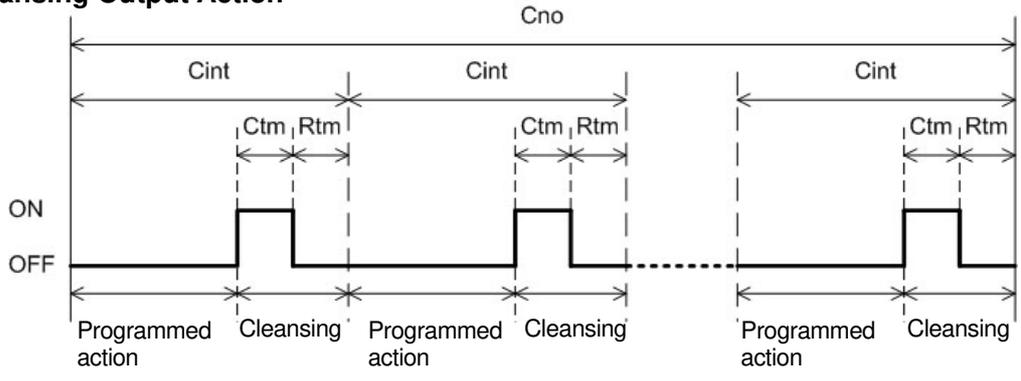

Cno: Number of cleansing cycles
 Cint: Cleansing interval
 Ctm: Cleansing time
 Rtm: Restore time after cleansing

(Fig. 8.4-2)

8.5 Zero/Slope Indication Group

To enter the Zero/Slope Indication group, follow the procedure below.

- ① $\bar{\bar{\bar{0}}}$ Press the key 4 times in pH/Temperature Display Mode, or Cleansing Output Mode.
- ② $\bar{\bar{\bar{E}}}$ Press the key.
 The unit enters the Zero/Slope Indication group, and the 'Zero indication' appears.

| Character | Setting Item, Function, Setting Range | Factory Default |
|--|--|-----------------|
| $\bar{\bar{\bar{E}}}$ $\square\square.00$ | Zero indication • Indicates potential difference when pH 7 is calibrated. However, if manual calibration is performed, zero indication value calculated at previous automatic calibration will not be updated. If calibration is not successfully completed, zero indication will show the value before calibration. • Indication range: Voltage equivalent to pH ± 1.5 | 0.0 mV |
| $\bar{\bar{\bar{4}}}$ $\square\square.2$ | Slope indication • From the voltage equivalent to the calibrated pH, electromotive force for the change of pH 1 will be indicated. If calibration is not successfully completed, slope indication will show the value before calibration. • Indication range: Voltage equivalent to pH 0.00 to 14.00 | 59.2 mV |

9. Calibration

The pH calibration mode, Temperature calibration mode, Transmission output 1 adjustment mode, and Transmission output 2 adjustment mode are described below.

9.1 pH Calibration Mode

For pH measurement using the glass electrode method, pH in the sensor location, electrode performance and standard solution accuracy respectively play an important role for obtaining reliable data.

There are 2 methods in pH calibration: Automatic Calibration and Manual Calibration

When *Auto* (Automatic) is selected in [pH Calibration Auto/Manual (p.31)], pH will be automatically calibrated.

When *Manu* (Manual) is selected in [pH Calibration Auto/Manual (p.31)], pH will be calibrated manually.

When *NoTE* (No Temperature Compensation) is selected in [Electrode RTD (p.28)], calibration will be automatically performed at 25°C basis.

Perform pH calibration while pH measured value is in a stable status.

The unit cannot enter pH calibration mode in the following cases:

- When *Lock 1*, *Lock 2* or *Lock 3* is selected in [Set value lock (p.29)].
- When *Cleansing* (Cleansing output) is selected in any one of [A11, A12, A21, A22 type (pp.21, 22)], and cleansing action is performing using the 'Cleansing time' and 'Restore time after cleansing' settings.

9.1.1 Automatic Calibration

The 1st point standard solution [pH 7 (JIS or US standard)] selected in [pH 7 calibration standard (p.20)] is automatically calibrated first. Then, the 2nd point standard solution [any one of pH 2, pH 4, pH 9 or pH 10 (JIS)] selected in [2nd Solution (p.20)] is calibrated.

The pH value (based on JIS Z8802) at each temperature of pH standard solution to be calibrated will be automatically calculated.

The following outlines the procedure for automatic calibration.

(1) The 1st Point Calibration

- ① Immerse the pH Combined Electrode Sensor in the 1st point standard solution (pH 7).
When selecting *Last value HOLD* in [Transmission output 1 status when calibrating (p.31)] or [Transmission output 2 status when calibrating] (p.31)], select it while the pH Combined Electrode Sensor is being immersed in the solution currently calibrated.
After that, immerse the pH Combined Electrode Sensor in the 1st point standard solution (pH 7).

- ② Press and hold the  key and  key (in that order) together for 3 seconds in pH/Temperature Display Mode, or Cleansing Output Mode.

The unit enters pH calibration mode, and indicates the following.

| Display | Indication |
|---------------------|-------------|
| pH Display | pH |
| Temperature Display | <i>PH 7</i> |

- ③ Press the  key.

Automatic calibration of the 1st point starts.

During Automatic calibration, pH on the pH Display flashes.

Automatic calibration is carried out using the Automatic electrode quality evaluation function (*).

When flashing stops, automatic calibration of the 1st point is complete.

(*) Depending on the selection in [pH 7 calibration standard (p.20)], the value calibrated by the Automatic electrode quality evaluation function will be as follows.

| pH7 Calibration Standard | Value Calibrated by the Automatic Electrode Quality Evaluation Function |
|--------------------------|---|
| JIS | pH 6.86 |
| US standard | pH 7.00 |

(2) The 2nd Point Calibration

- ① Confirm that automatic calibration of the 1st point is complete, then press the  key. The 2nd standard solution will be shown on the display as follows.

| Display | Indication |
|---------------------|--|
| pH Display | pH |
| Temperature Display | pH standard solution selected in [2nd Solution (p.20)] |

- ② Rinse the electrode, and immerse the pH Combined Electrode Sensor in the 2nd Standard solution.
- ③ Press the  key.
Automatic calibration for the 2nd point starts.
During Automatic calibration, pH on the pH Display flashes.
Automatic calibration is carried out using the Automatic electrode quality evaluation function.
When flashing stops, automatic calibration of the 2nd point will be complete.
- ④ Confirm that automatic calibration of the 2nd point is complete, then press the  key. The newly calibrated values will be applied to the unit, indicated as follows.

| Display | Indication |
|---------------------|-------------|
| pH Display | <i>cal</i> |
| Temperature Display | <i>Good</i> |

pH automatic calibration is now complete.

- ⑤ Press the  key.
The unit reverts to pH/Temperature Display Mode, or Cleansing Output Mode.

9.1.2 Manual Calibration

Manual calibration can be carried out using 2 types of solution with a difference of pH 2 or more.

The following outlines the procedure for manual calibration.

(1) The 1st Point Calibration

- ① Immerse the pH Combined Electrode Sensor in the 1st standard solution.
When selecting *BEFH* (Last value HOLD) in [Transmission output 1 status when calibrating (p.31)] or [Transmission output 2 status when calibrating] (p.31)], select it while the pH Combined Electrode Sensor is being immersed in the solution currently calibrated.
After that, immerse the pH Combined Electrode Sensor in the 1st point standard solution.

- ② Press and hold the  key and  key (in that order) together for 3 seconds in pH/Temperature Display Mode, or Cleansing Output Mode.
The unit enters pH calibration mode, and indicates the following.

| Display | Indication |
|---------------------|---|
| pH Display | pH is flashing. |
| Temperature Display |  |

- ③ Press the  key.
The unit enters the 1st point manual calibration mode, and indicates the following.

| Display | Indication |
|---------------------|---|
| pH Display |  and pH are indicated alternately. |
| Temperature Display | The calibrated value is indicated. |

- ④ Set the calibration value with the  or  key while checking the pH.
pH calibration value setting range: -7.00 to 7.00

- ⑤ Press the  key.
The 1st point calibration is completed, and indicates the following.

| Display | Indication |
|---------------------|---|
| pH Display | pH is flashing. |
| Temperature Display |  |

(2) The 2nd Point Calibration

- ① Rinse the electrode, and immerse the pH Combined Electrode Sensor in the 2nd Standard solution.

- ② Press the  key.
The 2nd point can be calibrated manually, indicated as follows.

| Display | Indication |
|---------------------|---|
| pH Display |  and pH are indicated alternately. |
| Temperature Display | The calibration value is indicated. |

- ③ Set the calibration value with the  or  key while checking the pH.
pH calibration value setting range: -7.00 to 7.00

- ④ Press the  key.
The 2nd point calibration is completed. The newly calibrated values will be applied to the unit, indicated as follows.

| Display | Indication |
|---------------------|-------------|
| pH Display | <i>CAL</i> |
| Temperature Display | <i>Good</i> |

Now, pH manual calibration is complete.

- ⑤ Press the  key.
The unit reverts to pH/Temperature Display Mode, or Cleansing Output Mode.

9.1.3 Error Code during pH Calibration

During pH calibration, if pH calibration cannot be performed due to unstable pH input or temperature compensation error, etc., the error code (Table 9.1.3-1) will flash on the Temperature Display.

(Table 9.1.3-1)

| Error Code | Error Type | Error | Description | Occurrence |
|------------|------------|--|--|-------------------------------|
| E11 | Error | Response Speed Error | When calibrating, the response of the pH Combined Electrode Sensor is slow. When the difference between the input and each of the 1st and 2nd solutions are within pH ± 1.50 , and input fluctuation is over pH ± 0.05 (in 10 seconds of assessment cycles) for 5 minutes, this is assumed to be an error. However, if input fluctuation is less than or equal to pH ± 0.05 , this is assumed to be within the normal range. | When calibrating |
| E12 | Error | Electrode Sensitivity Error | When calibrating, sensitivity of the pH Combined Electrode Sensor has deteriorated. The difference between 1st and 2nd standard solution value after calibration is less than or equal to pH 2.00. | |
| E13 | Error | Asymmetry Potential Error | When calibrating pH 7, the difference in electromotive force between the sensor-measured value and standard value exceeds the equivalent of pH ± 1.50 . | |
| E14 | Error | Standard Solution Error | The specified standard solution has not been used. When pH ± 1.50 is exceeded for the 1st and 2nd solutions. | |
| E15 | Error | Solution Temperature Error | When temperature is 55°C or more at pH 10 solution. | |
| E21 | Fail | Temperature Sensor Burnout | Temperature sensor lead wire is burnt out. | When measuring or calibrating |
| E22 | Fail | Temperature Sensor Short-circuited | Temperature sensor lead wire is short-circuited. | |
| E23 | Error | Outside Temperature Compensation Range | Measured temperature has exceeded 110.0°C. | |
| E24 | Error | Outside Temperature Compensation Range | Measured temperature is less than 0.0°C. | |

9.2 Temperature Calibration Mode

To calibrate a temperature, set a temperature calibration value.

If $\overline{NO\ COMP}$ (No temperature compensation) is selected in [Electrode RTD (p.28)], Temperature calibration mode is not available.

The unit cannot enter Temperature calibration mode in the following cases:

- When $\overline{LOCK 1}$ (Lock 1), $\overline{LOCK 2}$ (Lock 2) or $\overline{LOCK 3}$ (Lock 3) is selected in [Set value lock (p.29)].
- When \overline{CLEAN} (Cleansing output) is selected in any one of [A11, A12, A21, A22 type (pp.21, 22)], and cleansing action is performing using the 'Cleansing time' and 'Restore time after cleansing' settings.

When a sensor cannot be set at the exact location where measurement is desired, the resulting measured temperature may deviate from the temperature in the desired location. In this case, the desired temperature can be set for the desired location by setting a temperature calibration value. However, it is effective within the input rated range regardless of the temperature calibration value. Temperature after calibration = Current temperature + (Temperature calibration value)

(e.g.) When current temperature is 23.5°C,

If temperature calibration value is set to 1.5°C: $23.5 + (1.5) = 25.0^\circ\text{C}$

If temperature calibration value is set to -1.5°C: $23.5 + (-1.5) = 22.0^\circ\text{C}$

The following outlines the procedure for Temperature calibration.

- ① Press and hold the  key and  key (in that order) together for 3 seconds in pH/Temperature Display Mode, or Cleansing Output Mode.

The unit will proceed to Temperature calibration mode, and indicates the following.

| Display | Indication |
|---------------------|--|
| pH Display | \overline{pH} and temperature are indicated alternately. |
| Temperature Display | Temperature calibration value is indicated. |

- ② Set a temperature calibration value with the  or  key while checking the temperature. Setting range: -10.0 to 10.0°C (The placement of the decimal point does not follow the selection. It is fixed.)
- ③ Press the  key.

Temperature calibration is complete, and the unit reverts to pH/Temperature Display Mode, or Cleansing Output Mode.

9.3 Transmission Output 1 Adjustment Mode

Fine adjustment of Transmission output 1 is performed.

The instrument is adjusted at the factory, however, differences may occur between the indication value of the connected equipment (recorders, etc.) and output value of this instrument.

In this case, perform Transmission output 1 Zero adjustment and Span adjustment.

Transmission output 1 adjustment mode is available only when the Transmission output 1 (TA option) or Transmission output 2 (TA2 option) is ordered.

The unit cannot enter Transmission output 1 Zero adjustment mode in the following cases.

- During pH calibration or temperature calibration
- When $LOC 1$ (Lock 1), $LOC 2$ (Lock 2) or $LOC 3$ (Lock 3) is selected in [Set value lock (p.29)].
- When $CLEAN$ (Cleansing output) is selected in any one of [A11, A12, A21, A22 type (pp.21, 22)], and cleansing action is performing using the 'Cleansing time' and 'Restore time after cleansing' settings.

The following outlines the procedure for Transmission output 1 adjustment.

- ① Press and hold the  and  key (in that order) together for approx. 3 seconds in pH/Temperature Display Mode, or Cleansing Output Mode.

The unit enters Transmission output 1 Zero adjustment mode, and indicates the following.

| Display | Indication |
|---------------------|---|
| pH Display | $AUE 1$ |
| Temperature Display | Transmission output 1 Zero adjustment value |

- ② Set the Transmission output 1 Zero adjustment value with the  or  key, while viewing the value indicated on the connected equipment (recorders, etc.).

Setting range: $\pm 5.00\%$ of Transmission output 1 Span

- ③ Press the  key.

The unit enters Transmission output 1 Span adjustment mode, and indicates the following.

| Display | Indication |
|---------------------|---|
| pH Display | $AU 1$ |
| Temperature Display | Transmission output 1 Span adjustment value |

- ④ Set the Transmission output 1 Span adjustment value with the  or  key, while viewing the value indicated on the connected equipment (recorders, etc.).

Setting range: $\pm 5.00\%$ of Transmission output 1 Span

- ⑤ Press the  key.

The unit reverts to the Transmission output 1 Zero adjustment mode.

Repeat steps ② to ⑤ if necessary.

- ⑥ To finish Transmission output 1 adjustment, press the  key in Transmission output 1 Span adjustment mode.

The unit reverts to pH/Temperature Display Mode, or Cleansing Output Mode.

9.4 Transmission Output 2 Adjustment Mode

Fine adjustment of Transmission output 2 is performed.

The instrument is adjusted at the factory, however, differences may occur between the indication value of the connected equipment (recorders, etc.) and output value of this instrument.

In this case, perform Transmission output 2 Zero adjustment and Span adjustment.

Transmission output 2 adjustment mode is available only when Transmission output 2 (TA2 option) is ordered.

The unit cannot enter Transmission output 2 Zero adjustment mode in the following cases.

- During pH calibration or temperature calibration
- When $LOC 1$ (Lock 1), $LOC 2$ (Lock 2) or $LOC 3$ (Lock 3) is selected in [Set value lock (p.29)].
- When $CLEAN$ (Cleansing output) is selected in any one of [A11, A12, A21, A22 type (pp.21, 22)], and cleansing action is performing using the 'Cleansing time' and 'Restore time after cleansing' settings.

The following outlines the procedure for Transmission output 2 adjustment.

- ① Press and hold the  and  key (in that order) together for approx. 3 seconds in pH/Temperature Display Mode, or Cleansing Output Mode.

The unit enters Transmission output 2 Zero adjustment mode, and indicates the following.

| Display | Indication |
|---------------------|---|
| pH Display | AJZ |
| Temperature Display | Transmission output 2 Zero adjustment value |

- ② Set the Transmission output 2 Zero adjustment value with the  or  key, while viewing the value indicated on the connected equipment (recorders, etc.).

Setting range: $\pm 5.00\%$ of Transmission output 2 Span

- ③ Press the  key.

The unit enters Transmission output 2 Span adjustment mode, and indicates the following.

| Display | Indication |
|---------------------|---|
| pH Display | $AJ4$ |
| Temperature Display | Transmission output 2 Span adjustment value |

- ④ Set the Transmission output 2 Span adjustment value with the  or  key, while viewing the value indicated on the connected equipment (recorders, etc.).

Setting range: $\pm 5.00\%$ of Transmission output 2 Span

- ⑤ Press the  key.

The unit reverts to the Transmission output 2 Zero adjustment mode.

Repeat steps ② to ⑤ if necessary.

- ⑥ To finish the Transmission output 2 adjustment, press the  key in Transmission output 2 Span adjustment mode.

The unit reverts to pH/Temperature Display Mode, or Cleansing Output Mode.

10. Measurement

10.1 Starting Measurement

After mounting to the control panel, and wiring, setup and calibration are complete, turn the power to the instrument ON.

For approx. 4 seconds after the power is switched ON, the input characters are indicated on the pH Display and Temperature Display.

Depending on the input specification, indication on the Temperature Display differs as follows.

Pt spec

| pH Display | Temperature Display | Item Selected in [Electrode RTD (p.28)] | Item Selected in [Pt100 input wire type (p.28)] |
|------------|---------------------|---|---|
| PH□□ | Unlit | none: No temperature compensation | |
| | PT 10 | PT 10: Pt1000 | |
| | PT 02 | PT □□: Pt100 | PT 02: 2-wire type |
| | PT 03 | | PT 03: 3-wire type |

Cu spec

| pH Display | Temperature Display | Item selected in [Electrode RTD (p.28)] |
|------------|---------------------|---|
| PH□□ | Unlit | none: No temperature compensation |
| | CU 50 | CU 50: Cu500 |

During this time, all outputs are in OFF status, and LED indicators except the PWR Indicator turns off. After that, measurement starts, indicating the item selected in [Display selection (p.32)].

10.2 A□□ Output


When PH_L (pH input low limit action), PH_H (pH input high limit action), T_LPL (Temperature input low limit action) or T_HPH (Temperature input high limit action) is selected in [A11, A12, A21, A22 type (pp.21, 22)], the A□□ output is turned ON if measured value drops below or exceeds the A□□ value.

When $PHHL$ (pH input High/Low limits independent action) or T_HHL (Temperature input High/Low limits independent action) is selected in [A11, A12, A21, A22 type (pp.21, 22)], the alarm output is turned ON if the measured value exceeds A□□ High/Low limits independent upper side band, or drops below A□□ High/Low limits independent lower side band.

A1 or A2 output is turned ON depending on the settings in [A1, A2 output allocation (p.32)] and [Output ON time/OFF time when A1/A2 output ON (p.33)].

If Output ON time and OFF time are set, A1 or A2 output can be turned ON/OFF in a configured cycle when A1 or A2 output is ON. (Fig. 10.2-1)

Timing chart (Output ON time and OFF time when A1 output is ON)

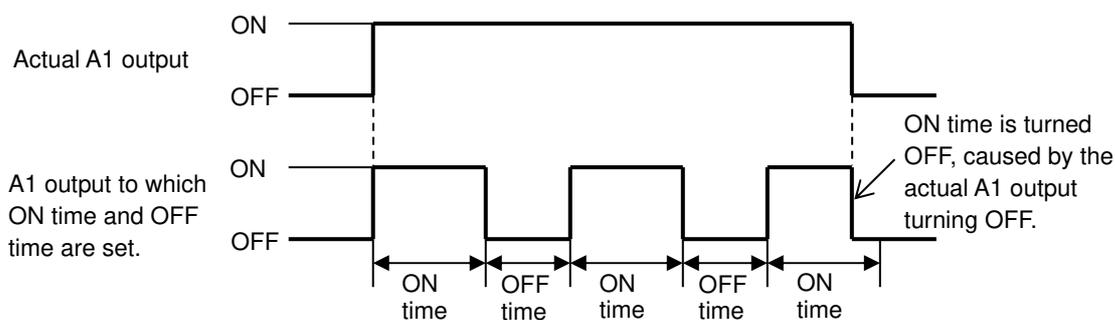

(Fig. 10.2-1)

A□□ output status can be read by reading Status flag 2 (A11, A12, A21, A22 output flag bit) in Serial communication.

A□□ output status, when input errors occur, differs depending on the selection in [A□□ output when input errors occur (p.27)].

- If \overline{OFF} (Disabled) is selected in [A□□ output when input errors occur (p.27)], A□□ output and A□□ output status will be turned OFF when input errors occur.
- If \overline{ON} (Enabled) is selected in [A□□ output when input errors occur (p.27)], A□□ output and A□□ output status will be maintained when input errors occur.
- If \overline{NOC} (No temperature compensation) is selected in [Electrode RTD (p.28)] selection, Temperature input low limit and Temperature input high limit actions will be disabled.

10.3 pH Input Error Alarm

pH input error alarm is used for detecting actuator trouble.

Even if pH input error alarm time has elapsed – if the change in pH input is smaller than the pH input error alarm band – the instrument assumes that actuator trouble has occurred, and sets Status flag 2 (A1, A2 pH input error alarm output flag bit).

In Serial communication, status can be read by reading Status flag 2 (A1, A2 pH input error alarm output flag bit).

pH input error alarm is enabled only when $\overline{PH_L}$ (pH input low limit alarm) $\overline{PH_H}$ (pH input high limit alarm) is selected in [A11, A12, A21, A22 type (p.21, 22)].

pH input error alarm is disabled during pH calibration.

10.4 Error Output

If \overline{ERR} (Error output) is selected in [A11, A12, A21, A22 type (pp. 21, 22)], the A1 or A2 output will be turned ON when error type is “Error”. See (Table 9.1.3-1, p.41).

10.5 Fail Output

If \overline{FAIL} (Fail output) is selected in [A11, A12, A21, A22 type (pp. 21, 22)], the A1 or A2 output will be turned ON when error type is “Fail”. See (Table 9.1.3-1, p.41).

10.6 Cleansing Output

If \overline{CLEAN} (Cleansing output) is selected in any one of [A11, A12, A21, A22 type (pp. 21, 22)], the unit will enter Cleansing Output Mode.

The A□□ output (for which the cleansing output is selected) will turn ON during the configured cleansing time.

When the cleansing interval finishes after restore time has passed, this is counted as one cleansing cycle, and the configured the number of cleansing cycles will be repeated.

While cleansing is being performed using the ‘Cleansing Time’ and ‘Restore Time after Cleansing’ settings, other outputs are in OFF status.

Measured values (pH, temperature) are constantly updated.


When cleansing is not being performed, programmed operation continues.

When power is turned ON again, the unit starts cleansing action from the first cleansing cycle.

After the configured number of cleansing cycles are finished, the A□□ output (for which the cleansing output is selected) is turned OFF, and other outputs perform their operations selected in [A11, A12, A21, A22 type (p.21, 22)]. However, they are in Cleansing Output Mode.

If any output other than \overline{CLEAN} (Cleansing output) is selected in [A11, A12, A21, A22 type (pp.21, 22)], the unit will revert to pH/Temperature Display Mode.

• Cleansing Output Action

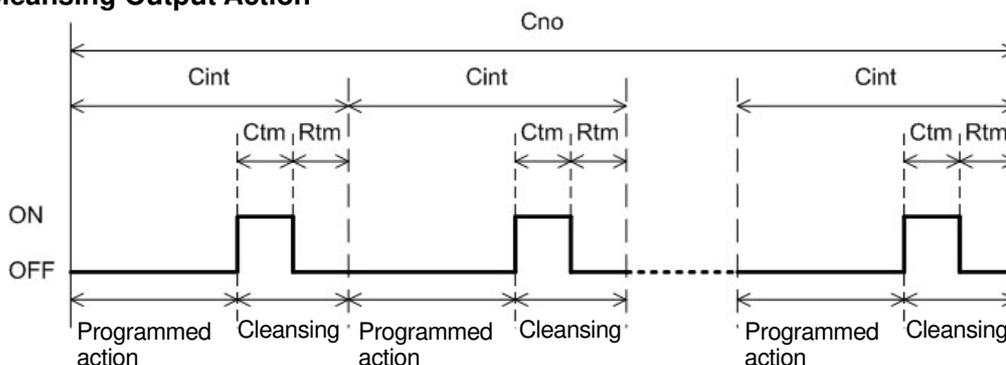

Cno: Number of cleansing cycles
 Cint: Cleansing interval
 Ctm: Cleansing time
 Rtm: Restore time after cleansing

(Fig. 10.6-1)

- While cleansing action is currently performing, if $cLE\bar{E}$ (Cleansing output) is selected in [A11, A12, A21, A22 type (p.21, 22)] again and it is allocated in [A1 output allocation] or [A2 output allocation], then the allocated output will be the same as the current cleansing output.
- If $n\bar{o}\bar{n}E$ (No temperature compensation) is selected in [Electrode RTD (p.28)], the value set in [Reference temperature] is maintained during cleansing action.
If an input error occurs [when temperature measured value is outside the measurement range (e.g.) less than 0.0°C or exceeding 110.0°C], the following will be displayed.

| pH Display | Temperature Display |
|-------------------|---------------------------------|
| pH measured value | Less than 0.0°C: $E\bar{E}24$ |
| pH measured value | Exceeding 110.0°C: $E\bar{E}23$ |

- During calibration mode, Transmission output 1 adjustment or Transmission output 2 adjustment, if cleansing action initiates after restore time has passed, the cleansing action will not be performed in the current session.
- If the number of cleansing cycles is changed in [Number of cleansing cycles] during cleansing action, the new number will be valid from the next cleansing cycle.

10.7 Manual Cleansing Mode

By pressing the \triangle and ∇ keys simultaneously for 3 seconds, the unit enters Manual Cleansing mode. In Manual Cleansing mode, cleansing action is performed using the 'Cleansing Time' and 'Restore Time after Cleansing' settings.

After cleansing is completed, the unit automatically reverts to Cleansing Output Mode.


During cleansing action, Manual cleansing via key operation is invalidated, so the unit cannot enter Manual cleansing mode.

During Manual cleansing mode, if programmed cleansing action initiates after Restore time has passed, the cleansing action will not be performed in the current session.

Cleansing action by Manual cleansing mode is also counted as 1 cleansing cycle.

If Lock 1, Lock 2 or Lock 3 is selected in [Set value lock], the unit cannot enter the Manual Cleansing mode.

Manual Cleansing Mode Action

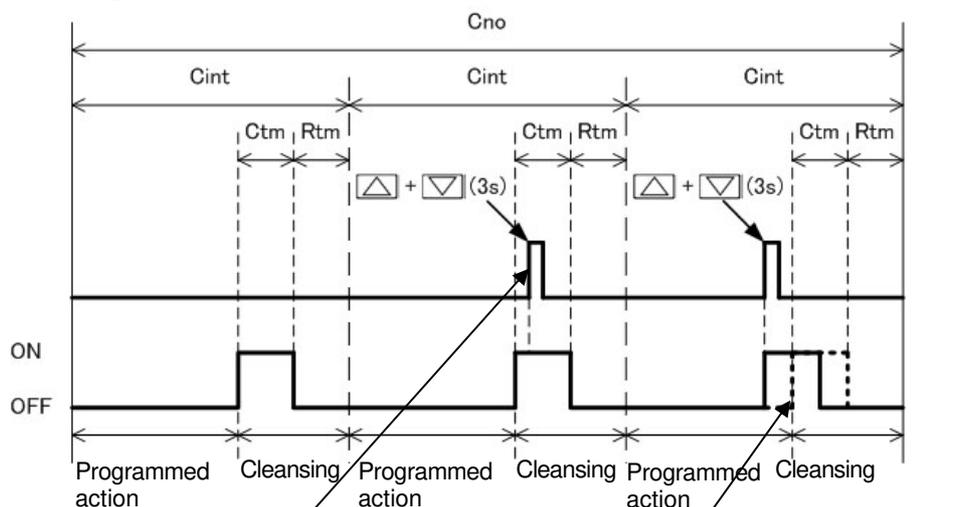

During cleansing action, Manual cleansing mode via key operation is invalidated – programmed cleansing mode takes priority.

During Manual cleansing mode, the programmed cleansing action will be invalidated. Cleansing action by Manual cleansing mode is counted as one cleansing cycle.

Cno: Number of cleansing cycles
Cint: Cleansing interval
Ctm: Cleansing time
Rtm: Restore time after cleansing

(Fig. 10.7-1)

10.8 Error Code during Measurement

For temperature sensor error or outside temperature compensation range during measurement, their corresponding error codes flash on the Temperature Display as shown below in (Table 10.8-1).

(Table 10.8-1)

| Error Code | Error Type | Error | Description | Occurrence |
|------------|------------|--|--|-------------------------------|
| EE21 | Fail | Temperature sensor burnout | Temperature sensor lead wire is burnt out. | When measuring or calibrating |
| EE22 | Fail | Temperature sensor short-circuited | Temperature sensor lead wire is short-circuited. | |
| EE23 | Error | Outside temperature compensation range | Measured temperature has exceeded 110.0°C. | |
| EE24 | Error | Outside temperature compensation range | Measured temperature is less than 0.0°C. | |

10.9 Transmission Output 1 and 2

Converting pH or temperature to analog signal every input sampling period, outputs in current.
(Factory default: Transmission output 1: pH, Transmission output 2: Temperature)

If *NONC* (No temperature compensation) is selected in [Electrode RTD (p.28)], and *TEMP* (Temperature transmission) is selected in [Transmission output 1 type (p.30)] or [Transmission output 2 type (p.30)], the value set in [Reference temperature (p.28)] will be output.

If Transmission output 1 high limit and low limit are set to the same value, Transmission output 1 will be fixed at 4 mA DC.

If Transmission output 2 high limit and low limit are set to the same value, Transmission output 2 will be fixed at 4 mA DC.

| | |
|-----------------|--|
| Resolution | 12000 |
| Current | 4 to 20 mA DC (Load resistance: Max 550 Ω) |
| Output accuracy | Within ±0.3% of Transmission output 1 Span or Transmission output 2 Span |

10.10 pH Fluctuation Alarm Output

pH fluctuation alarm output is used for detecting pH input fluctuation error.

Even if pH fluctuation alarm time has elapsed – if the change in pH input fluctuation is smaller than the pH fluctuation alarm band – the instrument assumes that a pH fluctuation error has occurred, and sets Status flag 2 (A11, A12, A21, A22 output flag bit).

If *EPHA* (pH fluctuation alarm output) is selected in [A11, A12, A21, A22 type (pp.21, 22)], the selected A□□ output will be turned ON.


In Serial communication, status can be read by reading Status flag 2 (A11, A12, A21, A22 output flag bit).

This function will be disabled if pH fluctuation alarm time is set to 0 (zero) hours, or if pH fluctuation alarm band is set to pH 0.00.

11. Communication


11.1 System Configuration Example

When Using USB Communication Cable CMC-001-3 (sold separately)

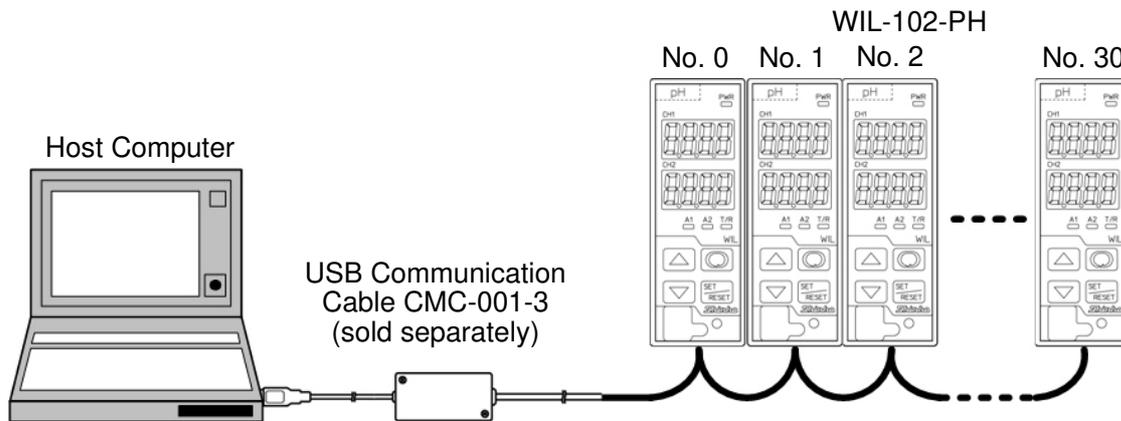

(Fig. 11.1-1)

When Using Communication Converter IF-400 (sold separately)

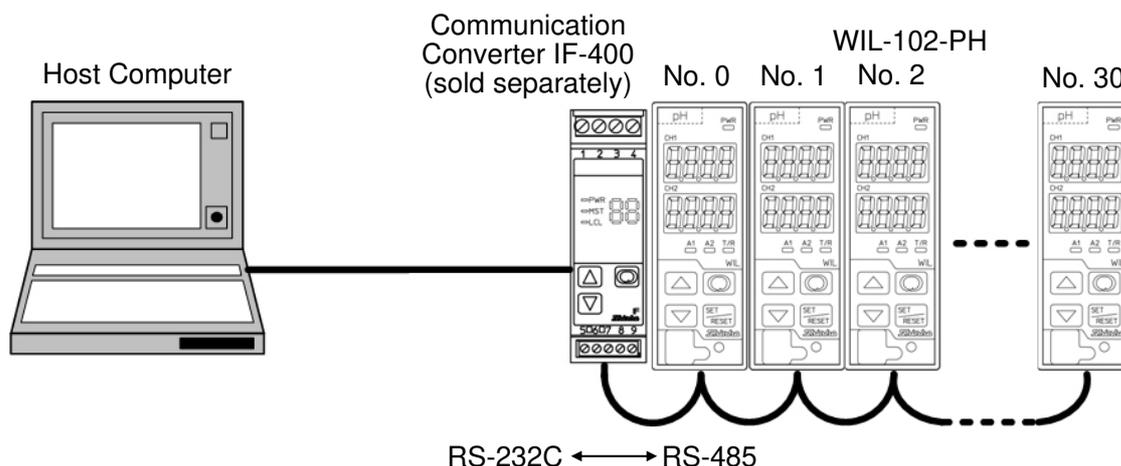

(Fig. 11.1-2)

11.2 Setting Method of the pH Meter

Communication parameters can be set in the Basic Function group.

To enter the Basic Function group, follow the procedure below.

- ① *afEr* Press the key 3 times in pH/Temperature Display Mode, or Cleansing Output Mode.
- ② *cnL* Press the key twice. 'Communication Protocol' appears.
- ③ Set each item. (Use the or key for settings, and register the value with the key.)


| Character | Setting Item, Function, Setting Range | Factory Default |
|--------------------------|--|-----------------|
| <i>cnL</i> <i>noL</i> | Communication protocol • Selects the communication protocol. • <i>noL</i> : Shinko protocol <i>nodr</i> : MODBUS ASCII mode <i>nodr</i> : MODBUS RTU mode | Shinko protocol |
| <i>cnno</i> | Instrument number • Sets the instrument number. The instrument numbers should be set one by one when multiple instruments are connected in Serial communication, otherwise communication is impossible. • Setting range: 0 to 95 | 0 |

| Character | Setting Item, Function, Setting Range | Factory Default |
|--------------|--|-----------------|
| cā4P □□96 | Communication speed • Selects a communication speed equal to that of the host computer. • □□96 : 9600 bps □ 192 : 19200 bps □384 : 38400 bps | 9600 bps |
| cāFF 7EEn | Data bit/Parity • Selects data bit and parity. • 8non : 8 bits/No parity 7non : 7 bits/No parity 8EEn : 8 bits/Even 7EEn : 7 bits/Even 8odd : 8 bits/Odd 7odd : 7 bits/Odd | 7 bits/Even |
| cā4f □□□1 | Stop bit • Selects the stop bit. • □□□1 : 1 bit □□□2 : 2 bits | 1 bit |

- ④ Press the  key multiple times. The unit reverts to pH/Temperature Display Mode, or Cleansing Output Mode.

11.3 Communication Procedure

Communication starts with command transmission from the host computer (hereafter Master) and ends with the response of the WIL-102-PH (hereafter Slave).

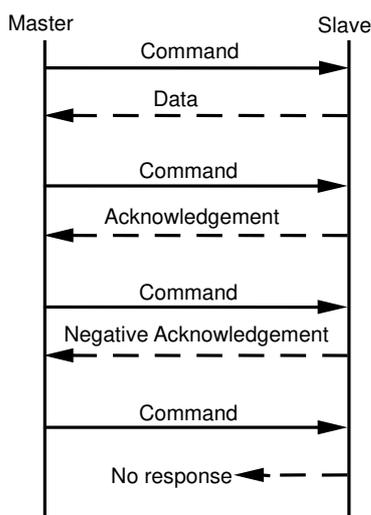

(Fig.11.3-1)

• Response with Data

When the master sends the reading command, the slave responds with the corresponding set value or current status.

• Acknowledgement

When the master sends the setting command, the slave responds by sending acknowledgement after processing is terminated.

• Negative Acknowledgement

When the master sends a non-existent command or value out of the setting range, the slave returns a negative acknowledgement.

• No Response

The slave will not respond to the master in the following cases:

- Global address (Shinko protocol) is set.
- Broadcast address (MODBUS protocol) is set.
- Communication error (framing error, parity error)
- Checksum error (Shinko protocol), LRC discrepancy (MODBUS ASCII mode), CRC-16 discrepancy (MODBUS RTU mode)

Communication Timing of the RS-485

Master Side (Take note while programming)

When the master starts transmission through the RS-485 communication line, the master is arranged so as to provide an idle status (mark status) transmission period of 1 or more character before sending the command to ensure synchronization on the receiving side.

Set the program so that the master can disconnect the transmitter from the communication line within a 1-character transmission period after sending the command in preparation for reception of the response from the slave.

To avoid collision of transmissions between the master and the slave, send the next command after carefully checking that the master has received the response.

If a response to the command is not returned due to communication errors, set the Retry Processing to send the command again. (It is recommended to execute Retry twice or more.)

Slave Side

When the slave starts transmission through the RS-485 communication line, the slave is arranged so as to provide an idle status (mark status) transmission period of 1 or more characters before sending the response to ensure synchronization on the receiving side.

The slave is arranged so as to disconnect the transmitter from the communication line within a 1-character transmission period after sending the response.

11.4 Shinko Protocol

11.4.1 Transmission Mode

Shinko protocol is composed of ASCII.

Hexadecimal (0 to 9, A to F), which is divided into high order (4-bit) and low order (4-bit) out of 8-bit binary data in command is transmitted as ASCII characters.

Data format Start bit: 1 bit
 Data bit: 7 bits
 Parity: Even
 Stop bit: 1 bit

Error detection: Checksum

11.4.2 Command Configuration

All commands are composed of ASCII.

The data (set value, decimal number) is represented by hexadecimal numbers.

The negative numbers are represented in 2's complement.

Numerals written below the command represent the number of characters.

(1) Setting Command

| | | | | | | | |
|-----------------|---------|----------------------|-----------------------|--------------|------|----------|--------------------|
| Header (02H) | Address | Sub address (20H) | Command type (50H) | Data item | Data | Checksum | Delimiter (03H) |
| 1 | 1 | 1 | 1 | 4 | 4 | 2 | 1 |

(Fig. 11.4.2-1)

(2) Reading Command

| | | | | | | |
|-----------------|---------|----------------------|-----------------------|--------------|----------|--------------------|
| Header (02H) | Address | Sub address (20H) | Command type (20H) | Data item | Checksum | Delimiter (03H) |
| 1 | 1 | 1 | 1 | 4 | 2 | 1 |

(Fig. 11.4.2-2)

(3) Response with Data

| | | | | | | | |
|-----------------|---------|----------------------|-----------------------|--------------|------|----------|--------------------|
| Header (06H) | Address | Sub address (20H) | Command type (20H) | Data item | Data | Checksum | Delimiter (03H) |
| 1 | 1 | 1 | 1 | 4 | 4 | 2 | 1 |

(Fig. 11.4.2-3)

(4) Acknowledgement

| | | | |
|-----------------|---------|----------|--------------------|
| Header (06H) | Address | Checksum | Delimiter (03H) |
| 1 | 1 | 2 | 1 |

(Fig. 11.4.2-4)

(5) Negative Acknowledgement

| | | | | |
|-----------------|---------|---------------|----------|--------------------|
| Header (15H) | Address | Error code | Checksum | Delimiter (03H) |
| 1 | 1 | 1 | 2 | 1 |

(Fig. 11.4.2-5)

Header: Control code to represent the beginning of the command or the response.
 ASCII codes are used.

Setting command, Reading command: STX (02H) fixed

Response with data, Acknowledgement: ACK (06H) fixed

Negative acknowledgement: NAK (15H) fixed

Instrument Number (Address): Numbers by which the master discerns each slave.

Instrument number 0 to 94 and Global address 95.

ASCII codes (20H to 7FH) are used by adding 20H to instrument numbers 0 to 95 (00H to 5FH).

95 (7FH) is called Global address, which is used when the same command is sent to all the slaves connected. However, the response is not returned.

Sub Address: 20H fixed

Command Type: Code to discern Setting command (50H) and Reading command (20H)

Data Item: Classification of the command object.

Composed of 4-digit hexadecimal numbers, using ASCII.

[Refer to "11.6. Communication Command Table". (pp. 57 to 65)]

- Data:** The contents of data (set value) differ depending on the setting command.
Composed of 4-digit hexadecimal numbers, using ASCII.
[Refer to “11.6. Communication Command Table”. (pp. 57 to 65)]
- Checksum:** 2-character data to detect communication errors.
Refer to “11.4.3 Checksum Calculation”.
- Delimiter:** Control code to represent the end of command.
ASCII code ETX (03H) fixed
- Error Code:** Represents an error type using ASCII.
1 (31H)-----Non-existent command
2 (32H)-----Not used
3 (33H)-----Setting outside the setting range
4 (34H)-----Status unable to be set (e.g. While Automatic electrode quality evaluation function is performing.)
5 (35H)-----During setting mode by keypad operation

11.4.3 Checksum Calculation

Checksum is used to detect receiving errors in the command or data.

Set the program for the master side as well to calculate the checksum of the response data from the slaves so that communication errors can be checked.

The ASCII code (hexadecimal) corresponding to the characters which range from the address to that before the checksum is converted to binary notation, and the total value is calculated.


The lower one byte of the total value is converted to 2's complement, and then to hexadecimal numbers, that is, ASCII code for the checksum.

- 1's complement: Reverse each binary bit. 0 will become 1 and vice versa.
- 2's complement: Add 1 to 1's complement.

Checksum Calculation Example

pH calibration value: 1.00 (0064H)

Address (instrument number): 0 (20H)

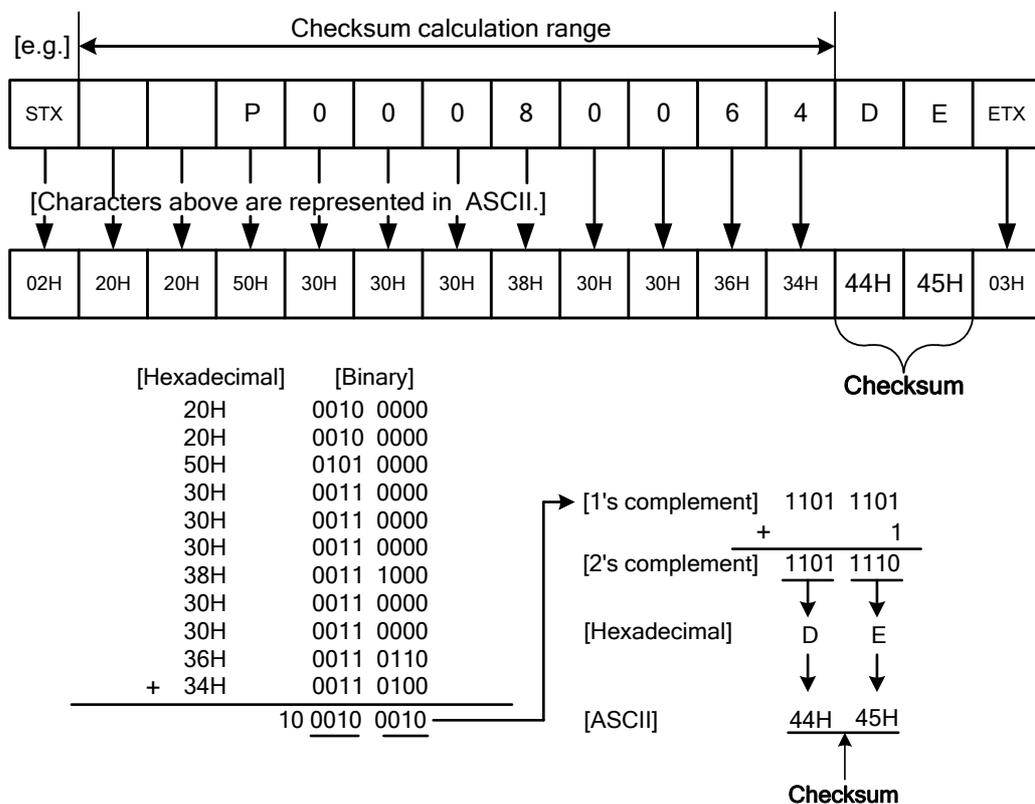

(Fig. 11.4.3-1)

11.5 MODBUS Protocol

11.5.1 Transmission Mode

There are 2 transmission modes (ASCII and RTU) in MODBUS protocol.

ASCII Mode

Hexadecimal (0 to 9, A to F), which is divided into high order (4-bit) and low order (4-bit) out of 8-bit binary data in command is transmitted as ASCII characters.

Data format Start bit: 1 bit
 Data bit: 7 bits (8 bits) (Selectable)
 Parity: Even (No parity, Odd) (Selectable)
 Stop bit: 1 bit (2 bits) (Selectable)

Error detection : LRC (Longitudinal Redundancy Check)

RTU Mode

8-bit binary data in command is transmitted as it is.

Data format Start bit: 1 bit
 Data bit: 8 bits
 Parity: No parity (Even, Odd) (Selectable)
 Stop bit: 1 bit (2 bits) (Selectable)

Error detection: CRC-16 (Cyclic Redundancy Check)

11.5.2 Data Communication Interval

ASCII Mode

Max.1 second of interval between ASCII mode characters

RTU Mode

Communication speed 9600 bps, 19200 bps:

To transmit continuously, an interval between characters which consist of one message, must be within 1.5-character transmission times.

Communication speed 38400 bps:

To transmit continuously, an interval between characters which consist of one message, must be within 750 μ s.

If an interval lasts longer than 1.5-character transmission times or 750 μ s, the WIL-102-PH assumes that transmission from the master is finished, which results in a communication error, and will not return a response.

11.5.3 Message Configuration

ASCII Mode

ASCII mode message is configured to start by Header [:(colon)(3AH)] and end by Delimiter [CR (carriage return) (0DH) + LF (Line feed)(0AH)].

| | | | | | | |
|---------------|------------------|------------------|------|--------------------|-------------------|-------------------|
| Header (:) | Slave address | Function Code | Data | Error check LRC | Delimiter (CR) | Delimiter (LF) |
|---------------|------------------|------------------|------|--------------------|-------------------|-------------------|

RTU Mode

Communication speed 9600 bps, 19200 bps: RTU mode is configured to start after idle time is processed for more than 3.5-character transmissions, and end after idle time is processed for more than 3.5-character transmissions.

Communication speed 38400 bps: RTU mode is configured to start after idle time is processed for more than 1.75 ms, and end after idle time is processed for more than 1.75 ms.

| | | | | | |
|------------------------|------------------|------------------|------|-----------------------|------------------------|
| 3.5 idle characters | Slave address | Function code | Data | Error check CRC-16 | 3.5 idle characters |
|------------------------|------------------|------------------|------|-----------------------|------------------------|

(1) Slave Address

Slave address is an individual instrument number on the slave side, and is set within the range 0 to 95 (00H to 5FH).

The master identifies slaves by the slave address of the requested message.

The slave informs the master which slave is responding to the master by placing its own address in the response message.

Slave address 00H (Broadcast address) can identify all the slaves connected. However, slaves do not respond.

(2) Function Code

The function code is the command code for the slave to undertake the following action types.

(Table 11.5.3-1)

| Function Code | Contents |
|---------------|---|
| 03 (03H) | Reading the set value and information from slaves |
| 06 (06H) | Setting to slaves |

Function code is used to discern whether the response is normal (acknowledgement) or if any error (negative acknowledgement) has occurred when the slave returns the response message to the master. When acknowledgement is returned, the slave simply returns the original function code. When negative acknowledgement is returned, the MSB of the original function code is set as 1 for the response.

(For example, when the master sends request message setting 10H to the function code by mistake, slave returns 90H by setting the MSB to 1, because the former is an illegal function.)

For negative acknowledgement, the exception codes below (Table 11.5.3-2) are set to the data of the response message, and returned to the master in order to inform it of what kind of error has occurred.

(Table 11.5.3-2)

| Exception Code | Contents |
|----------------|---|
| 1 (01H) | Illegal function (Non-existent function) |
| 2 (02H) | Illegal data address (Non-existent data address) |
| 3 (03H) | Illegal data value (Value out of the setting range) |
| 17 (11H) | Shinko protocol error code 4 [Status unable to be set (e.g.) Automatic electrode quality evaluation function is being performed.] |
| 18 (12H) | Shinko protocol error code 5 (During setting mode by keypad operation) |

(3) Data

Data differs depending on the function code.

A request message from the master is composed of data item, amount of data and setting data.

A response message from the slave is composed of the byte count, data and exception codes in negative acknowledgements, corresponding to the request message.

Effective range of data is -32768 to 32767 (8000H to 7FFFH).

(4) Error Check

ASCII Mode

After calculating LRC (Longitudinal Redundancy Check) from the slave address to the end of data, the calculated 8-bit data is converted to two ASCII characters, and are appended to the end of message.

How to Calculate LRC

- ① Create a message in RTU mode.
- ② Add all the values from the slave address to the end of data. This is assumed as X.
- ③ Make a complement for X (bit reverse). This is assumed as X.
- ④ Add a value of 1 to X. This is assumed as X.
- ⑤ Set X as an LRC to the end of the message.
- ⑥ Convert the whole message to ASCII characters.

RTU Mode

After calculating CRC-16 (Cyclic Redundancy Check) from the slave address to the end of the data, the calculated 16-bit data is appended to the end of message in sequence from low order to high order.

How to calculate CRC-16

In the CRC-16 system, the information is divided by the polynomial series. The remainder is added to the end of the information and transmitted. The generation of a polynomial series is as follows.

(Generation of polynomial series: $X^{16} + X^{15} + X^2 + 1$)

- ① Initialize the CRC-16 data (assumed as X) (FFFFH).
- ② Calculate exclusive OR (XOR) with the 1st data and X. This is assumed as X.
- ③ Shift X one bit to the right. This is assumed as X.

- ④ When a carry is generated as a result of the shift, XOR is calculated by X of ③ and the fixed value (A001H). This is assumed as X. If a carry is not generated, go to step ⑤.
- ⑤ Repeat steps ③ and ④ until shifting 8 times.
- ⑥ XOR is calculated with the next data and X. This is assumed as X.
- ⑦ Repeat steps ③ to ⑤.
- ⑧ Repeat steps ③ to ⑤ up to the final data.
- ⑨ Set X as CRC-16 to the end of message in sequence from low order to high order.

11.5.4 Message Example

ASCII Mode

Numerals written below the command represent the number of characters.

① Reading [Slave address 1, Data item 0080H (pH)]

- A request message from the master

Amount of data means how many data items are to be read. It is fixed as (30H 30H 30H 31H).

| | | | | | | |
|-----------------|----------------------------|----------------------------|---|--|------------------------------|------------------------|
| Header (3AH) | Slave Address (30H 31H) | Function Code (30H 33H) | Data Item [0080H] (30H 30H 38H 30H) | Amount of Data [0001H] (30H 30H 30H 31H) | Error Check LRC (37H 42H) | Delimiter (0DH 0AH) |
| 1 | 2 | 2 | 4 | 4 | 2 | 2 |

- Response message from the slave in normal status [pH 1.00 (0064H)]

The response byte count means the byte count of the data which has been read.

It is fixed as (30H 32H).

| | | | | | | |
|-----------------|----------------------------|----------------------------|---|--------------------------------------|------------------------------|------------------------|
| Header (3AH) | Slave Address (30H 31H) | Function Code (30H 33H) | Response Byte Count [02H] (30H 32H) | Data [0064H] (30H 30H 36H 34H) | Error Check LRC (39H 36H) | Delimiter (0DH 0AH) |
| 1 | 2 | 2 | 2 | 4 | 2 | 2 |

- Response message from the slave in exception (error) status (When a data item is incorrect)

The function code MSB is set to 1 for the response message in exception (error) status (83H).

The exception code 02H (Non-existent data address) is returned (error).

| | | | | | |
|-----------------|----------------------------|----------------------------|--------------------------------------|------------------------------|------------------------|
| Header (3AH) | Slave Address (30H 31H) | Function Code (38H 33H) | Exception Code [02H] (30H 32H) | Error Check LRC (37H 41H) | Delimiter (0DH 0AH) |
| 1 | 2 | 2 | 2 | 2 | 2 |

② Setting [Slave address 1, Data item 0008H (pH calibration value)]

- A request message from the master [When pH calibration value is set to 1.00 (0064H)]

| | | | | | | |
|-----------------|----------------------------|----------------------------|---|--------------------------------------|------------------------------|------------------------|
| Header (3AH) | Slave Address (30H 31H) | Function Code (30H 36H) | Data Item [0008H] (30H 30H 30H 38H) | Data [0064H] (30H 30H 36H 34H) | Error Check LRC (38H 44H) | Delimiter (0DH 0AH) |
| 1 | 2 | 2 | 4 | 4 | 2 | 2 |

- Response message from the slave in normal status

| | | | | | | |
|-----------------|----------------------------|----------------------------|---|--------------------------------------|------------------------------|------------------------|
| Header (3AH) | Slave Address (30H 31H) | Function Code (30H 36H) | Data Item [0008H] (30H 30H 30H 38H) | Data [0064H] (30H 30H 36H 34H) | Error Check LRC (38H 44H) | Delimiter (0DH 0AH) |
| 1 | 2 | 2 | 4 | 4 | 2 | 2 |

- Response message from the slave in exception (error) status (When a value out of the setting range is set)

The function code MSB is set to 1 for the response message in exception (error) status (86H).

The exception code 03H (Value out of the setting range) is returned (error).

| | | | | | |
|-----------------|----------------------------|----------------------------|--------------------------------------|------------------------------|------------------------|
| Header (3AH) | Slave Address (30H 31H) | Function Code (38H 36H) | Exception Code [03H] (30H 33H) | Error Check LRC (37H 36H) | Delimiter (0DH 0AH) |
| 1 | 2 | 2 | 2 | 2 | 2 |

RTU Mode

Numerals written below the command represent the number of characters.

① Reading [Slave address 1, Data item 0080H (pH)]

- A request message from the master

Amount of data means how many data items are to be read. It is fixed as (0001H).

| | | | | | | |
|---------------------|---------------------|---------------------|-------------------|------------------------|----------------------------|---------------------|
| 3.5 Idle Characters | Slave Address (01H) | Function Code (03H) | Data Item (0080H) | Amount of data (0001H) | Error Check CRC-16 (85E2H) | 3.5 idle characters |
| | 1 | 1 | 2 | 2 | 2 | |

- Response message from the slave in normal status [pH 1.00 (0064H)]

The response byte count means the byte count of the data which has been read.

It is fixed as (02H).

| | | | | | | |
|---------------------|---------------------|---------------------|---------------------------|--------------|----------------------------|---------------------|
| 3.5 Idle Characters | Slave Address (01H) | Function Code (03H) | Response Byte Count (02H) | Data (0064H) | Error Check CRC-16 (B9AFH) | 3.5 idle characters |
| | 1 | 1 | 1 | 2 | 2 | |

- Response message from the slave in exception (error) status (When data item is incorrect).
The function code MSB is set to 1 for the response message in exception (error) status (83H).

The exception code (02H: Non-existent data address) is returned (error).

| | | | | | |
|---------------------|---------------------|---------------------|----------------------|----------------------------|---------------------|
| 3.5 Idle Characters | Slave Address (01H) | Function Code (83H) | Exception Code (02H) | Error Check CRC-16 (C0F1H) | 3.5 idle characters |
| | 1 | 1 | 1 | 2 | |

② Setting [Slave address 1, Data item 0008H (pH calibration value)]

- A request message from the master [When pH calibration value is set to 1.00 (0064H)]

| | | | | | | |
|---------------------|---------------------|---------------------|-------------------|--------------|----------------------------|---------------------|
| 3.5 Idle Characters | Slave Address (01H) | Function Code (06H) | Data Item (0008H) | Data (0064H) | Error Check CRC-16 (D9E3H) | 3.5 idle characters |
| | 1 | 1 | 2 | 2 | 2 | |

- Response message from the slave in normal status

| | | | | | | |
|---------------------|---------------------|---------------------|-------------------|--------------|----------------------------|---------------------|
| 3.5 Idle Characters | Slave Address (01H) | Function Code (06H) | Data Item (0008H) | Data (0064H) | Error Check CRC-16 (D9E3H) | 3.5 idle characters |
| | 1 | 1 | 2 | 2 | 2 | |

- Response message from the slave in exception (error) status (When a value out of the setting range is set)

The function code MSB is set to 1 for the response message in exception (error) status (86H).

The exception code (03H: Value out of the setting range) is returned (error).

| | | | | | |
|---------------------|---------------------|---------------------|----------------------|----------------------------|---------------------|
| 3.5 Idle Characters | Slave Address (01H) | Function Code (86H) | Exception Code (03H) | Error Check CRC-16 (0261H) | 3.5 idle characters |
| | 1 | 1 | 1 | 2 | |

11.6 Communication Command Table

11.6.1 Notes about Setting/Reading Command

- The data (set value, decimal) is converted to hexadecimal numbers.
A negative number is represented in 2's complement.
- When connecting multiple slaves, the address (instrument number) must not be duplicated.
- Data items 0200H to 0209H (User save area 1 to 10) can be read or set in 1 word units.
Effective range of data is -32768 to 32767 (8000H to 7FFFH).
- MODBUS protocol uses Holding Register addresses. The Holding Register addresses are created as follows. A Shinko command data item is converted to decimal number, and the offset of 40001 is added.

The result is the Holding Register address.

Using Data item 0001H (2nd solution) as an example:

Data item in the sending message is 0001H, however, MODBUS protocol Holding Register address is 40002 (1 + 40001).

- Even if options are not ordered, setting or reading via software communication will be possible. Command contents of the A11, A12, A21, A22 will function, however, Transmission output 1 and Transmission output 2 command contents will not function.

(1) Setting Command

- Up to 1,000,000 (one million) entries can be stored in non-volatile IC memory. If the number of settings exceeds the limit, the data will not be saved. So, ensure the set values are not frequently changed via software communication. (If a value set via software communication is the same as the value before the setting, the value will not be written in non-volatile IC memory.)
- Be sure to select Lock 3 when changing the set value frequently via software communication. If Lock 3 is selected, all set values – except Electrode RTD, Temperature calibration value, pH calibration value, pH calibration Auto/Manual, Transmission output 1 Zero adjustment value, Transmission output 1 Span adjustment value, Transmission output 2 Zero adjustment value, Transmission output 2 Span adjustment value – can be temporarily changed. However, they revert to their previous value after the power is turned off because they are not saved in the non-volatile IC memory.
Do not change setting items (A11, A12, A21, A22 type). If they are changed, they will affect other setting items.
- Setting range of each item is the same as that of keypad operation.
- When the data (set value) has a decimal point, a whole number (hexadecimal) without a decimal point is used.
- If A11, A12, A21 or A22 type is changed at Data items 0003H (A11 type), 0050H (A12 type), 0051H (A21 type) or 0052H (A22 type), the A11, A12, A21 or A22 value will default to 0 (zero).
The output status of A11, A12, A21 or A22 will also be initialized.
- Settings via software communication are possible while in Set value lock status.
- Communication parameters such as Instrument Number, Communication Speed of the slave cannot be set by the software communication function. They can only be set via the keypad. (pp.49, 50)
- When sending a command by Global address [95 (7FH), Shinko protocol] or Broadcast address [00H, MODBUS protocol], the same command is sent to all the slaves connected. However, the response is not returned.

(2) Reading Command

- When the data (set value) has a decimal point, a whole number (hexadecimal) without a decimal point is used for a response.

11.6.2 Setting/Reading Command

| Shinko Command Type | MODBUS Function Code | Data Item | | Data | | | | | | | | | | | | | | | |
|---------------------|----------------------|---------------------|---------------------------------------|---|------|------------|---------------------|-------|----|-------------|-------|----|---------------|-------|---------------|-------------|-------|---------------|---------------|
| 50H/20H | 06H/03H | 0001H | 2nd solution | 0000H: pH 2 0001H: pH 4 0002H: pH 9 0003H: pH 10 | | | | | | | | | | | | | | | |
| 50H/20H | 06H/03H | 0002H | pH input decimal point place | 0000H: No decimal point 0001H: 1 digit after decimal point 0002H: 2 digits after decimal point | | | | | | | | | | | | | | | |
| 50H/20H | 06H/03H | 0003H | A11 type | 0000H: No action 0001H: pH input low limit action 0002H: pH input high limit action 0003H: Temperature input low limit 0004H: Temperature input high limit 0005H: Error output 0006H: Fail output 0007H: Cleansing output 0008H: pH fluctuation alarm output 0009H: pH input High/Low limits independent 000AH: Temperature input High/Low limits independent | | | | | | | | | | | | | | | |
| 50H/20H | 06H/03H | 0004H | A11 value | Set value | | | | | | | | | | | | | | | |
| 50H/20H | 06H/03H | 0005H | A11 ON side | Set value | | | | | | | | | | | | | | | |
| 50H/20H | 06H/03H | 0006H | A11 ON delay time | Set value | | | | | | | | | | | | | | | |
| 50H/20H | 06H/03H | 0007H | A11 OFF delay time | Set value | | | | | | | | | | | | | | | |
| 50H/20H | 06H/03H | 0008H | pH calibration value | Set value | | | | | | | | | | | | | | | |
| 50H/20H | 06H/03H | 0009H | pH 7 calibration standard | 0000H: JIS 0001H: US standard | | | | | | | | | | | | | | | |
| 50H/20H | 06H/03H | 0021H | Electrode RTD | Pt spec 0000H: No temperature compensation 0001H: Pt1000 0002H: Pt100 Cu spec 0000H: No temperature compensation 0001H: Cu500 | | | | | | | | | | | | | | | |
| 50H/20H | 06H/03H | 0022H | Temperature input decimal point place | 0000H: No decimal point 0001H: 1 digit after decimal point | | | | | | | | | | | | | | | |
| 50H/20H | 06H/03H | 0023H | Reference temperature | Set value | | | | | | | | | | | | | | | |
| 50H/20H | 06H/03H | 0028H | Temperature calibration value | Set value | | | | | | | | | | | | | | | |
| 50H/20H | 06H/03H | 0030H | Set value lock | 0000H: Unlock 0001H: Lock 1 0002H: Lock 2 0003H: Lock 3 | | | | | | | | | | | | | | | |
| 50H/20H | 06H/03H | 0031H | Transmission output 1 type | 0000H: pH transmission 0001H: Temperature transmission | | | | | | | | | | | | | | | |
| 50H/20H | 06H/03H | 0032H | Transmission output 1 high limit | Set value | | | | | | | | | | | | | | | |
| 50H/20H | 06H/03H | 0033H | Transmission output 1 low limit | Set value | | | | | | | | | | | | | | | |
| 50H/20H | 06H/03H | 0034H | pH calibration Auto/Manual | 0000H: Automatic 0001H: Manual | | | | | | | | | | | | | | | |
| 50H/20H | 06H/03H | 0035H | Auto-light function | 0000H: Disabled 0001H: Enabled | | | | | | | | | | | | | | | |
| 50H/20H | 06H/03H | 0036H | Display selection | <table border="1"> <thead> <tr> <th>Data</th> <th>pH Display</th> <th>Temperature Display</th> </tr> </thead> <tbody> <tr> <td>0000H</td> <td>pH</td> <td>Temperature</td> </tr> <tr> <td>0001H</td> <td>pH</td> <td>No indication</td> </tr> <tr> <td>0002H</td> <td>No indication</td> <td>Temperature</td> </tr> <tr> <td>0003H</td> <td>No indication</td> <td>No indication</td> </tr> </tbody> </table> | Data | pH Display | Temperature Display | 0000H | pH | Temperature | 0001H | pH | No indication | 0002H | No indication | Temperature | 0003H | No indication | No indication |
| Data | pH Display | Temperature Display | | | | | | | | | | | | | | | | | |
| 0000H | pH | Temperature | | | | | | | | | | | | | | | | | |
| 0001H | pH | No indication | | | | | | | | | | | | | | | | | |
| 0002H | No indication | Temperature | | | | | | | | | | | | | | | | | |
| 0003H | No indication | No indication | | | | | | | | | | | | | | | | | |

| Shinko Command Type | MODBUS Function Code | Data Item | | Data |
|---------------------|----------------------|-----------|------------------------------------|---|
| 50H/20H | 06H/03H | 0037H | Indication time | Set value |
| 50H | 06H | 0038H | pH calibration mode | 0000H: pH/Temperature Display Mode, or Cleansing Output Mode 0001H: Calibration mode |
| 50H | 06H | 0039H | pH calibration start | 0001H: 1st point calibration start 0002H: 1st point calibration complete 0003H: 2nd point calibration start 0004H: 2nd point calibration complete |
| 50H/20H | 06H/03H | 0040H | pH input filter time constant | Set value |
| 50H/20H | 06H/03H | 0041H | A□□ output when input errors occur | 0000H: Enabled 0001H: Disabled |
| 50H/20H | 06H/03H | 0042H | Cable length correction | Set value |
| 50H/20H | 06H/03H | 0043H | Cable cross-section area | Set value |
| 50H/20H | 06H/03H | 0048H | Output ON time when A1 output ON | Set value |
| 50H/20H | 06H/03H | 0049H | Output OFF time when A1 output ON | Set value |
| 50H/20H | 06H/03H | 004AH | Output ON time when A2 output ON | Set value |
| 50H/20H | 06H/03H | 004BH | Output OFF time when A2 output ON | Set value |
| 50H/20H | 06H/03H | 0050H | A12 type | 0000H: No action 0001H: pH input low limit action 0002H: pH input high limit action 0003H: Temperature input low limit 0004H: Temperature input high limit 0005H: Error output 0006H: Fail output 0007H: Cleansing output 0008H: pH fluctuation alarm output 0009H: pH input High/Low limits independent 000AH: Temperature input High/Low limits independent |
| 50H/20H | 06H/03H | 0051H | A21 type | 0000H: No action 0001H: pH input low limit action 0002H: pH input high limit action 0003H: Temperature input low limit 0004H: Temperature input high limit 0005H: Error output 0006H: Fail output 0007H: Cleansing output 0008H: pH fluctuation alarm output 0009H: pH input High/Low limits independent 000AH: Temperature input High/Low limits independent |
| 50H/20H | 06H/03H | 0052H | A22 type | 0000H: No action 0001H: pH input low limit action 0002H: pH input high limit action 0003H: Temperature input low limit 0004H: Temperature input high limit 0005H: Error output 0006H: Fail output 0007H: Cleansing output 0008H: pH fluctuation alarm output 0009H: pH input High/Low limits independent 000AH: Temperature input High/Low limits independent |

| Shinko Command Type | MODBUS Function Code | Data Item | | Data |
|---------------------|----------------------|-----------|--|---|
| 50H/20H | 06H/03H | 0053H | A12 value | Set value |
| 50H/20H | 06H/03H | 0054H | A21 value | Set value |
| 50H/20H | 06H/03H | 0055H | A22 value | Set value |
| 50H/20H | 06H/03H | 0056H | A12 ON side | Set value |
| 50H/20H | 06H/03H | 0057H | A21 ON side | Set value |
| 50H/20H | 06H/03H | 0058H | A22 ON side | Set value |
| 50H/20H | 06H/03H | 0059H | A12 ON delay time | Set value |
| 50H/20H | 06H/03H | 005AH | A21 ON delay time | Set value |
| 50H/20H | 06H/03H | 005BH | A22 ON delay time | Set value |
| 50H/20H | 06H/03H | 005CH | A12 OFF delay time | Set value |
| 50H/20H | 06H/03H | 005DH | A21 OFF delay time | Set value |
| 50H/20H | 06H/03H | 005EH | A22 OFF delay time | Set value |
| 50H/20H | 06H/03H | 0068H | pH input sensor correction | Set value |
| 50H/20H | 06H/03H | 0069H | Temperature Display when no temperature compensation | 0000H: Reference temperature 0001H: Unlit |
| 50H/20H | 06H/03H | 006AH | A1 output allocation | 0000H: A11 type 0001H: A12 type 0002H: A21 type 0003H: A22 type 0004H: A11, A12 types 0005H: A21, A22 types 0006H: A11, A21 types 0007H: A12, A22 types 0008H: A11, A12, A21, A22 types |
| 50H/20H | 06H/03H | 006BH | A2 output allocation | 0000H: A11 type 0001H: A12 type 0002H: A21 type 0003H: A22 type 0004H: A11, A12 types 0005H: A21, A22 types 0006H: A11, A21 types 0007H: A12, A22 types 0008H: A11, A12, A21, A22 types |
| 50H/20H | 06H/03H | 006FH | Pt100 input wire type | 0000H: 2-wire type 0001H: 3-wire type |
| 50H / 20H | 06H / 03H | 0070H | Reserved (*) | |
| 50H / 20H | 06H / 03H | 0071H | Reserved (*) | |
| 50H / 20H | 06H / 03H | 0072H | Reserved (*) | |
| 50H / 20H | 06H / 03H | 0073H | Reserved (*) | |
| 50H / 20H | 06H / 03H | 0074H | Reserved (*) | |
| 50H / 20H | 06H / 03H | 0075H | Reserved (*) | |
| 50H / 20H | 06H / 03H | 0076H | Reserved (*) | |
| 50H / 20H | 06H / 03H | 0077H | Reserved (*) | |
| 50H | 06H | 007FH | Key operation change flag clearing | 0001H: Clear change flag |

(*) If the reserved item is read, acknowledgement (undefined value) will be returned.
If the reserved item is set, the instrument action will be changed, so do not set this item.

| Shinko Command Type | MODBUS Function Code | Data Item | | Data |
|---------------------|----------------------|-----------|---|--|
| 50H/20H | 06H/03H | 0100H | A11 hysteresis type | 0000H: Medium Value 0001H: Reference Value |
| 50H/20H | 06H/03H | 0101H | A12 hysteresis type | 0000H: Medium Value 0001H: Reference Value |
| 50H/20H | 06H/03H | 0102H | A21 hysteresis type | 0000H: Medium Value 0001H: Reference Value |
| 50H/20H | 06H/03H | 0103H | A22 hysteresis type | 0000H: Medium Value 0001H: Reference Value |
| 50H/20H | 06H/03H | 0104H | A11 OFF side | Set value |
| 50H/20H | 06H/03H | 0105H | A12 OFF side | Set value |
| 50H/20H | 06H/03H | 0106H | A21 OFF side | Set value |
| 50H/20H | 06H/03H | 0107H | A22 OFF side | Set value |
| 50H/20H | 06H/03H | 0108H | Number of cleansing cycles | Set value |
| 50H/20H | 06H/03H | 0109H | Cleansing interval | Set value |
| 50H/20H | 06H/03H | 010AH | Cleansing time | Set value |
| 50H/20H | 06H/03H | 010BH | Restore time after cleansing | Set value |
| 50H | 06H | 010CH | Manual cleansing mode | 0001H: Manual cleansing mode |
| 50H/20H | 06H/03H | 010FH | Transmission output 1 status when calibrating | 0000H: Last value HOLD 0001H: Set value HOLD 0002H: Measured value |
| 50H/20H | 06H/03H | 0110H | Transmission output 1 value HOLD when calibrating | Set value |
| 50H/20H | 06H/03H | 0111H | A1 pH input error alarm A□□ type | 0000H: No action 0001H: A11 type 0002H: A12 type 0003H: A21 type 0004H: A22 type |
| 50H/20H | 06H/03H | 0112H | A2 pH input error alarm A□□ type | 0000H: No action 0001H: A11 type 0002H: A12 type 0003H: A21 type 0004H: A22 type |
| 50H/20H | 06H/03H | 0115H | A1 pH input error alarm band when A□□ output ON | Set value |
| 50H/20H | 06H/03H | 0116H | A1 pH input error alarm time when A□□ output ON | Set value |
| 50H/20H | 06H/03H | 0117H | A1 pH input error alarm band when A□□ output OFF | Set value |
| 50H/20H | 06H/03H | 0118H | A1 pH input error alarm time when A□□ output OFF | Set value |
| 50H/20H | 06H/03H | 0119H | A2 pH input error alarm band when A□□ output ON | Set value |
| 50H/20H | 06H/03H | 011AH | A2 pH input error alarm time when A□□ output ON | Set value |
| 50H/20H | 06H/03H | 011BH | A2 pH input error alarm band when A□□ output OFF | Set value |

| Shinko Command Type | MODBUS Function Code | Data Item | | Data |
|---------------------|----------------------|-----------|--|--|
| 50H/20H | 06H/03H | 011CH | A2 pH input error alarm time when A□□ output OFF | Set value |
| 50H/20H | 06H/03H | 0125H | pH input error alarm time unit | 0000H: Second(s) 0001H: Minute(s) |
| 50H | 06H | 0126H | Transmission output 1 adjustment mode | 0000H: pH/Temperature Display Mode, or Cleansing Output Mode 0001H: Transmission output 1 Zero adjustment mode 0002H: Transmission output 1 Span adjustment mode |
| 50H/20H | 06H/03H | 0127H | Transmission output 1 Zero adjustment value | Set value |
| 50H/20H | 06H/03H | 0128H | Transmission output 1 Span adjustment value | Set value |
| 50H/20H | 06H/03H | 0131H | A11 pH fluctuation alarm time | Set value |
| 50H/20H | 06H/03H | 0132H | A12 pH fluctuation alarm time | Set value |
| 50H/20H | 06H/03H | 0133H | A21 pH fluctuation alarm time | Set value |
| 50H/20H | 06H/03H | 0134H | A22 pH fluctuation alarm time | Set value |
| 50H/20H | 06H/03H | 0135H | A11 pH fluctuation alarm band | Set value |
| 50H/20H | 06H/03H | 0136H | A12 pH fluctuation alarm band | Set value |
| 50H/20H | 06H/03H | 0137H | A21 pH fluctuation alarm band | Set value |
| 50H/20H | 06H/03H | 0138H | A22 pH fluctuation alarm band | Set value |
| 50H/20H | 06H/03H | 0139H | A11 High/Low limits independent lower side band | Set value |
| 50H/20H | 06H/03H | 013AH | A12 High/Low limits independent lower side band | Set value |
| 50H/20H | 06H/03H | 013BH | A21 High/Low limits independent lower side band | Set value |
| 50H/20H | 06H/03H | 013CH | A22 High/Low limits independent lower side band | Set value |
| 50H/20H | 06H/03H | 013DH | A11 High/Low limits independent upper side band | Set value |
| 50H/20H | 06H/03H | 013EH | A12 High/Low limits independent upper side band | Set value |
| 50H/20H | 06H/03H | 013FH | A21 High/Low limits independent upper side band | Set value |
| 50H/20H | 06H/03H | 0140H | A22 High/Low limits independent upper side band | Set value |
| 50H/20H | 06H/03H | 0141H | A11 hysteresis | Set value |
| 50H/20H | 06H/03H | 0142H | A12 hysteresis | Set value |
| 50H/20H | 06H/03H | 0143H | A21 hysteresis | Set value |
| 50H/20H | 06H/03H | 0144H | A22 hysteresis | Set value |

| Shinko Command Type | MODBUS Function Code | Data Item | | Data |
|---------------------|----------------------|-----------|---|--|
| 50H/20H | 06H/03H | 0145H | Transmission output 1 status when cleansing | 0000H: Last value HOLD 0001H: Set value HOLD 0002H: Measured value |
| 50H/20H | 06H/03H | 0146H | Transmission output 1 value HOLD when cleansing | Set value |
| 50H/20H | 06H/03H | 0147H | Transmission output 2 type | 0000H: pH transmission 0001H: Temperature transmission |
| 50H/20H | 06H/03H | 0148H | Transmission output 2 high limit | Set value |
| 50H/20H | 06H/03H | 0149H | Transmission output 2 low limit | Set value |
| 50H | 06H | 014AH | Transmission output 2 adjustment mode (*) | 0000H: pH/Temperature display mode, or Cleansing output mode 0001H: Transmission output 2 Zero adjustment mode 0002H: Transmission output 2 Span adjustment mode |
| 50H/20H | 06H/03H | 014BH | Transmission output 2 Zero adjustment value | Set value |
| 50H/20H | 06H/03H | 014CH | Transmission output 2 Span adjustment value | Set value |
| 50H/20H | 06H/03H | 014DH | Transmission output 2 status when calibrating | 0000H: Last value HOLD 0001H: Set value HOLD 0002H: Measured value |
| 50H/20H | 06H/03H | 014EH | Transmission output 2 value HOLD when calibrating | Set value |
| 50H/20H | 06H/03H | 014FH | Transmission output 2 status when cleansing | 0000H: Last value HOLD 0001H: Set value HOLD 0002H: Measured value |
| 50H/20H | 06H/03H | 0150H | Transmission output 2 value HOLD when cleansing | Set value |
| 50H/20H | 06H/03H | 0151H | pH inputs for moving average | Set value |
| 50H/20H | 06H/03H | 0152H | Temperature inputs for moving average | Set value |
| 50H/20H | 06H/03H | 0200H | User save area 1 | -32768 to 32767 (8000H to 7FFFH) |
| 50H/20H | 06H/03H | 0201H | User save area 2 | -32768 to 32767 (8000H to 7FFFH) |
| 50H/20H | 06H/03H | 0202H | User save area 3 | -32768 to 32767 (8000H to 7FFFH) |
| 50H/20H | 06H/03H | 0203H | User save area 4 | -32768 to 32767 (8000H to 7FFFH) |
| 50H/20H | 06H/03H | 0204H | User save area 5 | -32768 to 32767 (8000H to 7FFFH) |
| 50H/20H | 06H/03H | 0205H | User save area 6 | -32768 to 32767 (8000H to 7FFFH) |
| 50H/20H | 06H/03H | 0206H | User save area 7 | -32768 to 32767 (8000H to 7FFFH) |
| 50H/20H | 06H/03H | 0207H | User save area 8 | -32768 to 32767 (8000H to 7FFFH) |
| 50H/20H | 06H/03H | 0208H | User save area 9 | -32768 to 32767 (8000H to 7FFFH) |
| 50H/20H | 06H/03H | 0209H | User save area 10 | -32768 to 32767 (8000H to 7FFFH) |

(*) If 'Setting' is executed while Transmission output 2 (TA2 option) is not ordered, the following error code will be returned.

- Shinko protocol: Error code 4 (34H)
- MODBUS: Exception code 17 (11H)

| Shinko Command Type | MODBUS Function Code | Data Item | | Data | | | | | | | | | | | | |
|---------------------|----------------------|---|---|-----------------|----------|--------|---|---|---|---|---|---|---|---|---|--|
| 20H | 03H | 0090H | Temperature | Temperature | | | | | | | | | | | | |
| 20H | 03H | 0091H | Status flag 2 0000 0000 0000 0000 2^{15} to 2^0 2^0 digit: Cleansing output 0: OFF 1: ON 2^1 digit: A2 output 0: OFF 1: ON 2^2 digit: Not used (Always 0) 2^3 digit: A11 output flag (*) 0: OFF 1: ON 2^4 digit: A12 output flag (*) 0: OFF 1: ON 2^5 digit: A21 output flag (*) 0: OFF 1: ON 2^6 digit: A22 output flag (*) 0: OFF 1: ON 2^7 digit: Cleansing action (Cleansing time) 0: During programmed action 1: During cleansing time 2^8 digit: Cleansing action (Restore time after cleansing) 0: During programmed action 1: During Restore time after cleansing 2^9 digit: Manual cleansing action status flag 0: No Manual cleansing action 1: During Manual cleansing action 2^{10} digit: Transmission output 2 Zero adjustment status flag 0: pH/Temperature Display Mode, or Cleansing Output Mode 1: During Transmission output 2 Zero adjustment in Transmission output 2 adjustment mode $2^{11}, 2^{12}$ digits: Transmission output 1 adjustment status flag <table border="1" style="margin-left: 20px;"> <thead> <tr> <th>2^{12}</th> <th>2^{11}</th> <th>Status</th> </tr> </thead> <tbody> <tr> <td>0</td> <td>0</td> <td>pH/Temperature Display Mode, or Cleansing Output Mode</td> </tr> <tr> <td>0</td> <td>1</td> <td>During Transmission output 1 Zero adjustment in Transmission output 1 adjustment mode</td> </tr> <tr> <td>1</td> <td>0</td> <td>During Transmission output 1 Span adjustment in Transmission output 1 adjustment mode</td> </tr> </tbody> </table> 2^{13} digit: A1 pH input error alarm output flag 0: OFF 1: ON 2^{14} digit: A2 pH input error alarm output flag 0: OFF 1: ON 2^{15} digit: Transmission output 2 Span adjustment status flag 0: pH/Temperature Display Mode, or Cleansing Output Mode 1: During Transmission output 2 Span adjustment in Transmission output 2 adjustment mode | 2^{12} | 2^{11} | Status | 0 | 0 | pH/Temperature Display Mode, or Cleansing Output Mode | 0 | 1 | During Transmission output 1 Zero adjustment in Transmission output 1 adjustment mode | 1 | 0 | During Transmission output 1 Span adjustment in Transmission output 1 adjustment mode | |
| 2^{12} | 2^{11} | Status | | | | | | | | | | | | | | |
| 0 | 0 | pH/Temperature Display Mode, or Cleansing Output Mode | | | | | | | | | | | | | | |
| 0 | 1 | During Transmission output 1 Zero adjustment in Transmission output 1 adjustment mode | | | | | | | | | | | | | | |
| 1 | 0 | During Transmission output 1 Span adjustment in Transmission output 1 adjustment mode | | | | | | | | | | | | | | |
| 20H | 03H | 010DH | Zero indication | Indicated value | | | | | | | | | | | | |
| 20H | 03H | 010EH | Slope indication | Indicated value | | | | | | | | | | | | |

(*) A□□ output flag:

When CLEAN (Cleansing output) is selected in [A11, A12, A21, A22 type]: The A□□ output flag changes to 1 (ON).

If any item other than CLEAN (Cleansing output) is selected in [A11, A12, A21, A22 type]:

When A□□ output is turned ON: The A□□ output flag changes to 1 (ON).

When A□□ output is turned OFF: The A□□ output flag changes to 0 (OFF).

11.7 pH Calibration, Transmission Output 1 and 2 Adjustment via Communication Command

Like a keypad operation, there are also 2 methods in pH Calibration via communication command:
Automatic Calibration and Manual Calibration.

Perform pH Calibration while pH measured value is in a stable status.

11.7.1 pH Calibration

(1) Automatic Calibration

Automatic Calibration is performed in sequence from the 1st standard solution pH 7 (JIS or US standard) selected at Data item 0009H (pH 7 calibration standard) first, and then the 2nd standard solution [any one of pH 2, pH 4, pH 9 or pH 10 (JIS)] selected at Data item 0001H (2nd solution). pH value (based on JIS Z8802) at each temperature of pH standard solution to be calibrated is automatically calculated.

The following outlines the procedure for Automatic Calibration.

• The 1st Point Automatic Calibration

- ① Immerse the pH Combined Electrode Sensor in the 1st standard solution (pH 7).
When selecting Last value HOLD (0000H) at Data item 010FH (Transmission output 1 status when calibrating) or 014DH (Transmission output 2 status when calibrating), select it while the pH Combined Electrode Sensor is being immersed in the solution currently calibrated.
After that, immerse the pH Combined Electrode Sensor in the 1st point standard solution (pH 7).
- ② Set Data item 0038H (pH calibration mode) to 0001H.
The unit proceeds to pH calibration mode.
- ③ Set Data item 0039H (pH calibration start) to 0001H.
The 1st point Automatic calibration starts.
- ④ If 2^{13} , 2^{12} digits are read at Data item 0081H (Status flag 1), 01 (During the 1st point calibration) will be returned during automatic calibration.
Automatic Calibration is performed using the Automatic electrode quality evaluation function.
- ⑤ If 2^{13} , 2^{12} digits are read at Data item 0081H (Status flag 1), 00 (Standby) will be returned after automatic calibration.
- ⑥ Set Data item 0039H (pH calibration start) to 0002H.
The 1st point automatic calibration is complete, and the unit moves to the 2nd point automatic calibration mode.

• The 2nd Point Automatic Calibration

- ① After the electrode is rinsed, immerse the pH Combined Electrode Sensor in the 2nd standard solution.
- ② Set Data item 0039H (pH calibration start) to 0003H.
Automatic calibration for the 2nd point starts.
- ③ If 2^{13} , 2^{12} digits are read at Data item 0081H (Status flag 1), 10 (During the 2nd point calibration) will be returned during automatic calibration.
Automatic calibration is performed using the Automatic electrode quality evaluation function.
- ④ If 2^{13} , 2^{12} digits are read at Data item 0081H (Status flag 1), 11 (Calibration complete) will be returned after automatic calibration.
- ⑤ Set Data item 0039H (pH calibration start) to 0004H.
Automatic calibration for the 2nd point is complete.
- ⑥ Set Data item 0038H (pH calibration mode) to 0000H.
The pH automatic calibration is complete, and the unit will revert to pH/Temperature Display Mode, or Cleansing Output Mode.

(2) Manual Calibration

When there is a difference of pH 2 or more, Manual Calibration can be performed using the randomly selected 2 kinds of solution.

The following outlines the procedure for Manual Calibration.

• The 1st Point Manual Calibration

- ① Immerse the pH Combined Electrode Sensor in the 1st standard solution.
When selecting Last value HOLD (0000H) at Data item 010FH (Transmission output 1 status when calibrating) or 014DH (Transmission output 2 status when calibrating), select it while the pH Combined Electrode Sensor is being immersed in the solution currently calibrated.
After that, immerse the pH Combined Electrode Sensor in the 1st point standard solution.
- ② Set Data item 0038H (pH calibration mode) to 0001H.
- ③ Set Data item 0039H (pH calibration start) to 0001H.
Manual calibration for the 1st point starts.
- ④ If 2^{13} , 2^{12} digits are read at Data item 0081H (Status flag 1), 01 (During the 1st point calibration) will be returned during manual calibration.
- ⑤ Set a pH calibration value at Data item 0008H (pH calibration value).
- ⑥ Set Data item 0039H (pH calibration start) to 0002H.
Manual calibration for the 1st point is complete, and the unit will enter the 2nd point Manual Calibration mode.
- ⑦ If 2^{13} , 2^{12} digits are read at Data item 0081H (Status flag 1), 00 (Standby) will be returned after manual calibration.

• The 2nd Point Manual Calibration

- ① Rinse the electrode, then immerse the pH Combined Electrode Sensor in the 2nd standard solution.
- ② Set Data item 0039H (pH calibration start) to 0003H.
Manual calibration for the 2nd point starts.
- ③ If 2^{13} , 2^{12} digits are read at Data item 0081H (Status flag 1), 10 (During the 2nd point calibration) will be returned during manual calibration.
- ④ Set a pH calibration value at Data item 0008H (pH calibration value).
- ⑤ Set Data item 0039H (pH calibration start) to 0004H.
Manual calibration for the 2nd point will be complete.
- ⑥ If 2^{13} , 2^{12} digits are read at Data item 0081H (Status flag 1), 11 (Calibration complete) will be returned after manual calibration.
- ⑦ Set Data item 0038H (pH calibration mode) to 0000H.
The pH Manual calibration is complete, and the unit will revert to pH/Temperature Display Mode, or Cleansing Output Mode.

(3) Error Code during pH Calibration

If pH calibration cannot be performed due to unstable pH input, temperature compensation error, etc., Error code 1 (Error, Burnout, Short-circuited, etc.) will be returned when 2^0 digit to 2^{10} digit at Data item 0081H (Status flag 1) are read.

To release the Error code, set Data item 0038H (pH calibration mode) to 0000H.

The unit will return to pH/Temperature Display Mode, or Cleansing Output Mode.

If Data item 0039H (pH calibration start) is set during pH calibration of the 1st or 2nd point, the following error code will be returned.

Shinko protocol: Error code 34H

MODBUS protocol: Exception code 11H

11.7.2 Transmission Output 1 Adjustment

Fine adjustment of Transmission output 1 is performed.

The pH meter is adjusted at the factory, however, differences may occur between the indication value of the connected equipment (recorders, etc.) and the output value of this instrument. In this case, perform Transmission output 1 Zero adjustment and Span adjustment.

The following outlines the procedure for Transmission output 1 adjustment.

- ① Set Data item 0126H (Transmission output 1 adjustment mode) to 0001H.
The unit moves to Transmission output 1 Zero adjustment mode.
If 2¹² and 2¹¹ digits are read at Data item 0091H (Status flag 2), 01 (During Transmission output 1 Zero adjustment in Transmission output 1 adjustment mode) will be returned.
- ② Set the Transmission output 1 Zero adjustment value at Data item 0127H (Transmission output 1 Zero adjustment value), while viewing the value indicated on the connected equipment (recorders, etc.).
Setting range: $\pm 5.00\%$ of Transmission output 1 Span
- ③ Set Data item 0126H (Transmission output 1 adjustment mode) to 0002H.
The unit moves to Transmission output 1 Span adjustment mode.
If 2¹² and 2¹¹ digits are read at Data item 0091H (Status flag 2), 10 (During Transmission output 1 Span adjustment in Transmission output 1 adjustment mode) will be returned.
- ④ Set Transmission output 1 Span adjustment value at Data item 0128H (Transmission output 1 Span adjustment value), while viewing the value indicated on the connected equipment (recorders, etc.).
Setting range: $\pm 5.00\%$ of Transmission output 1 Span
- ⑤ Repeat steps ① to ④ if necessary.
- ⑥ To finish the Transmission output 1 adjustment, set Data item 0126H (Transmission output 1 adjustment mode) to 0000H.
The unit reverts to pH/Temperature Display Mode, or Cleansing Output Mode.

11.7.3 Transmission Output 2 Adjustment

Fine adjustment of Transmission output 2 is performed.

The pH meter is adjusted at the factory, however, differences may occur between the indication value of the connected equipment (recorders, etc.) and the output value of this instrument. In this case, perform Transmission output 2 Zero adjustment and Span adjustment.

The following outlines the procedure for Transmission output 2 adjustment.

- ① Set Data item 014AH (Transmission output 2 adjustment mode) to 0001H.
The unit moves to Transmission output 2 Zero adjustment mode.
If 2¹⁰ digit is read at Data item 0091H (Status flag 2), 1 (During Transmission output 2 Zero adjustment in Transmission output 2 adjustment mode) will be returned.
- ② Set the Transmission output 2 Zero adjustment value at Data item 014BH (Transmission output 2 Zero adjustment value), while viewing the value indicated on the connected equipment (recorders, etc.).
Setting range: $\pm 5.00\%$ of Transmission output 2 Span
- ③ Set Data item 014AH (Transmission output 2 adjustment mode) to 0002H.
The unit moves to Transmission output 2 Span adjustment mode.
If 2¹⁵ digit is read at Data item 0091H (Status flag 2), 1 (During Transmission output 2 Span adjustment in Transmission output 2 adjustment mode) will be returned.
- ④ Set Transmission output 2 Span adjustment value at Data item 014CH (Transmission output 2 Span adjustment value), while viewing the value indicated on the connected equipment (recorders, etc.).
Setting range: $\pm 5.00\%$ of Transmission output 2 Span
- ⑤ Repeat steps ① to ④ if necessary.
- ⑥ To finish the Transmission output 2 adjustment, set Data item 014AH (Transmission output 2 adjustment mode) to 0000H.
The unit reverts to pH/Temperature Display Mode, or Cleansing Output Mode.

11.8 Notes on Programming Monitoring Software

11.8.1 How to Speed up the Scan Time

When monitoring multiple units of the WIL-102-PH, set the program so that the requisite minimum pieces of data such as Data item 0080H (pH), Data item 0090H (Temperature), Data item 0081H (Status flag 1), Data item 0091H (Status flag 2) can be read. For other data, set the program so that they can be read only when their set value has been changed. This will speed up the scan time.

11.8.2 How to Read the Set Value Changes Made by Front Keypad Operation

If any set value is changed by keypad operation, the instrument sets [0081H (Status flag 1) 2¹⁵: Change in key operation] to 1 (Yes).

There are 2 methods of reading the set value changes made by the front keypad:

(1) Reading Method 1

- ① On the monitoring software side, check that [0081H (Status flag 1) 2¹⁵: Change in key operation] has been set to 1 (Yes), then read all set values.
- ② Clear [0081H (Status flag 1) 2¹⁵: Change in key operation], by setting Data item 007FH (Key operation change flag clearing) to 0001H (Clear change flag).
If Data item 007FH (Key operation change flag clearing) is set to 0001H (Clear change flag) during the setting mode of the instrument, Error code 5 (35H, Shinko protocol) or Exception Code 18 (12H, MODBUS protocol) will be returned as a negative acknowledgement. And [0081H (Status flag 1) 2¹⁵: Change in key operation] cannot be cleared.
Set a program so that all set values can be read when a negative acknowledgement is returned.
- ③ Read all set values again after acknowledgement is returned.

(2) Reading Method 2

- ① On the monitoring software side, check that [0081H (Status flag 1) 2¹⁵: Change in key operation] has been set to 1 (Yes), then set Data item 007FH (Key operation change flag clearing) to 0001H (Clear change flag).
- ② Set the program depending on the acknowledgement or negative acknowledgement as follows.

When acknowledgement is returned:

Consider it as settings completed, and read all set values.

When Error code 5 (35H, Shinko protocol) or Exception code 18 (12H, MODBUS protocol) is returned as a negative acknowledgement:

Consider it as still in setting mode, and read the requisite minimum pieces of data such as Data items 0080H (pH), 0090H (Temperature), 0081H (Status flag 1), 0091H (Status flag 2), then return to step ①.

Thus, programs which do not affect the scan time can be created using the methods described above, even if set values on the monitoring software will not be updated until settings are complete.

11.8.3 Note when Sending All Set Values Simultaneously

- If A11, A12, A21 or A22 type is changed at Data items 0003H (A11 type), 0050H (A12 type), 0051H (A21 type) or 0052H (A22 type), the A11, A12, A21 or A22 value will default to 0 (zero). Output status of A11, A12, A21 or A22 will also be initialized.

First, send the A11, A12, A21, A22 type, then send the A11, A12, A21, A22 value set at Data items 0004H (A11 value), 0053H (A12 value), 0054H (A21 value) and 0055H (A22 value).

12. Specifications

12.1 Standard Specifications

Rating

| Rated scale | Input | | Input Range | Resolution |
|----------------------|---|--------------------------|---------------------|---------------------|
| | pH combined electrode | | pH 0.00 to 14.00 | pH 0.01 |
| | Pt spec | Pt1000 | 0.0 to 100.0°C | 0.1°C |
| | | Pt100 | 0.0 to 100.0°C | 0.1°C |
| Cu spec | Cu500/25°C | 0.0 to 100.0°C | 0.1°C | |
| Input | pH Combined Electrode Sensor (pH sensor: JIS Z8802 Temperature element: Pt1000 or Pt100) pH Combined Electrode Sensor (pH sensor: JIS Z8802 Temperature element: Cu500/25°C) | | | |
| Power supply voltage | Model | WIL-102-PH | | WIL-102-PH 1 |
| | Power supply voltage | 100 to 240 V AC 50/60 Hz | 24 V AC/DC 50/60 Hz | |
| | Allowable voltage fluctuation range | 85 to 264 V AC | 20 to 28 V AC/DC | |

General Structure

| | | | |
|----------------------|---|---|--|
| External dimensions | 30 x 88 x 108 mm (W x H x D, including socket) | | |
| Mounting | DIN rail | | |
| Case | Material: Flame-resistant resin, Color: Light gray | | |
| Panel | Membrane sheet | | |
| Indication structure | Display | | |
| | pH Display | Red LED 4-digits, character size 10 x 4.6 mm (H x W) | |
| | Temperature Display | Red LED 4-digits, character size 10 x 4.6 mm (H x W) | |
| | Action indicator | | |
| | PWR (Yellow) | Lit when power supply is ON. | |
| | A1 (Red) | Lit when A1 output is ON. (Unlit when TA2 option is added) | |
| | A2 (Yellow) | Lit when A2 output is ON. (Unlit when TA option or TA2 option is added) | |
| | T/R (Yellow) | Lit while in Serial communication TX output (transmitting) | |
| Setting structure | Setting method: Input system using membrane sheet key | | |

Indication Performance

| | |
|---------------------------------|------------------------------------|
| Repeatability | pH value: pH ± 0.05 |
| Linearity | pH value: pH ± 0.05 |
| Temperature indication accuracy | Temperature: $\pm 1^\circ\text{C}$ |
| Input sampling period | 125 ms (2 inputs) |
| Time accuracy | Within $\pm 1\%$ of setting time |

Standard Functions

| | |
|-------------------------|--|
| pH calibration | <p>For pH measurement using the glass electrode method, pH in the sensor location, electrode performance and standard solution accuracy respectively play an important role for obtaining reliable data. 2-points calibration is performed using the standard solutions. However, it is effective within the input rated range regardless of the calibration value.</p> <p>There are 2 calibration methods: Automatic Calibration, Manual Calibration.</p> |
| Temperature calibration | <p>When a sensor cannot be set at the exact location where measurement is desired, the resulting measured temperature may deviate from the temperature in the desired location. In this case, the desired temperature can be set for the desired location by setting a temperature calibration value. However, it is effective within the input rated range regardless of the temperature calibration value.</p> |

| | | | | |
|------------------------|--|------------------------|-----------------------------------|-----------------------------------|
| Serial communication | The following operations can be carried out from an external computer. (1) Reading and setting of various set values (2) Reading of the pH, temperature and status (3) Function change, adjustment (4) Reading and setting of user save area | | | |
| Cable length | 1.2 km (Max.), Cable resistance: Within 50 Ω (Terminators are not necessary, but if used, use 120 Ω or more on one side.) | | | |
| Communication line | EIA RS-485 | | | |
| Communication method | Half-duplex communication | | | |
| Communication speed | 9600, 19200, 38400 bps (Selectable by keypad) | | | |
| Synchronization method | Start-stop synchronization | | | |
| Code form | ASCII, Binary | | | |
| Communication protocol | Shinko protocol, MODBUS ASCII, MODBUS RTU (Selectable by keypad) | | | |
| Data bit/Parity | 8 bits/No parity, 7 bits/No parity, 8 bits/Even, 7 bits/Even, 8 bits/Odd, 7 bits/Odd (Selectable by keypad) | | | |
| Stop bit | 1 bit, 2 bits (Selectable by keypad) | | | |
| Error correction | Command request repeat system | | | |
| Error detection | Parity check, Checksum (Shinko protocol), LRC (MODBUS protocol ASCII), CRC-16 (MODBUS protocol RTU) | | | |
| Data format | Communication Protocol | Shinko Protocol | MODBUS ASCII | MODBUS RTU |
| | Start bit | 1 | 1 | 1 |
| | Data bit | 7 | 7 (8) Selectable | 8 |
| | Parity | Even | Even (No parity, Odd), Selectable | No parity (Even, Odd), Selectable |
| | Stop bit | 1 | 1 (2), Selectable | 1 (2), Selectable |

Insulation/Dielectric Strength

| | |
|----------------------------------|--|
| Circuit insulation configuration | <p style="text-align: center;">[] : When the corresponding option is ordered</p> <p style="text-align: center;">Insulation Resistance: 10 MΩ minimum, at 500 V DC</p> |
| Dielectric strength | <p>Between power terminal - ground: 1.5 kV AC for 1 minute</p> <p>Between input terminal - ground: 1.5 kV AC for 1 minute</p> <p>Between input terminal - power terminal: 1.5 kV AC for 1 minute</p> |

Attached Functions

| Set value lock | <p>$L o c 1$ (Lock 1): None of the set values can be changed. $L o c 2$ (Lock 2): Only A11, A12, A21, A22 values can be changed. $L o c 3$ (Lock 3): All set values – except Electrode RTD, Temperature calibration value, pH calibration value, pH calibration Auto/Manual, Transmission output 1 Zero adjustment value, Transmission output 1 Span adjustment value, Transmission output 2 Zero adjustment value, Transmission output 2 Span adjustment value – can be temporarily changed. However, they revert to their previous value after the power is turned off because they are not saved in the non-volatile IC memory.</p> | | | | | | | | | | | | | | | | | | |
|--|---|------------|---------------------|-------------------------|--|---------------------------|--|------------|---------------------|--------------------------------------|-------------|--|-------------|------------|---------------------|----|---------------------------------|----|-----------------------------------|
| pH input sensor correction | <p>pH value measured by the pH Combined Electrode Sensor may deviate from the pH value in the measured location. In this case desired pH value can be obtained by adding a sensor correction value. However, it is effective within the measurement range regardless of the sensor correction value.</p> | | | | | | | | | | | | | | | | | | |
| Temperature Display when no temperature compensation | <p>If 'Reference temperature' is selected in [Temperature Display when no temperature compensation], the value set in [Reference temperature] will be indicated on the Temperature Display. If 'Unlit' is selected, the Temperature Display will turn off. If 'Temperature transmission' is selected in [Transmission output 1 type] or [Transmission output 2 type], the value set in [Reference temperature] will be output.</p> | | | | | | | | | | | | | | | | | | |
| Outside measurement range | <p>If pH measured value or temperature measured value is outside the measurement range, the following will be indicated. However, if pH measured value is outside the measurement range, and when the unit proceeds to pH calibration mode, the pH Display will turn off, and the Temperature Display will flash $\square F \square \square$. If temperature measured value is outside the measurement range, and when the unit proceeds to pH calibration mode, the pH Display will turn off, and the Temperature Display will flash an error code.</p> <p>pH measured value is outside the measurement range: If the value is less than pH 0.00 or exceeds pH 14.00, the following will be indicated.</p> <ul style="list-style-type: none"> When $n o n E$ (No temperature compensation) is selected in [Electrode RTD (p.28)] <table border="1" data-bbox="512 1400 1481 1518"> <thead> <tr> <th data-bbox="512 1400 1026 1440">pH Display</th> <th data-bbox="1026 1400 1481 1440">Temperature Display</th> </tr> </thead> <tbody> <tr> <td data-bbox="512 1440 1026 1480">Less than pH 0.00: 0.00</td> <td data-bbox="1026 1440 1481 1480">$\square F \square \square$ is flashing.</td> </tr> <tr> <td data-bbox="512 1480 1026 1518">Exceeding pH 14.00: 14.00</td> <td data-bbox="1026 1480 1481 1518">$\square F \square \square$ is flashing.</td> </tr> </tbody> </table> <ul style="list-style-type: none"> With Pt spec, when $P t 10$ (Pt1000) or $P t \square$ (Pt100) is selected in [Electrode RTD (p.28)] With Cu spec, when $C u 5 \square$ (Cu500) is selected in [Electrode RTD (p.28)] <table border="1" data-bbox="512 1691 1481 1809"> <thead> <tr> <th data-bbox="512 1691 1026 1731">pH Display</th> <th data-bbox="1026 1691 1481 1731">Temperature Display</th> </tr> </thead> <tbody> <tr> <td data-bbox="512 1731 1026 1771">Less than pH 0.00: 0.00 is flashing.</td> <td data-bbox="1026 1731 1481 1771">Temperature</td> </tr> <tr> <td data-bbox="512 1771 1026 1809">Exceeding pH 14.00: 14.00 is flashing.</td> <td data-bbox="1026 1771 1481 1809">Temperature</td> </tr> </tbody> </table> <p>If temperature measured value is outside the measurement range (Less than 0.0°C or exceeding 110.0°C), the following will be indicated.</p> <table border="1" data-bbox="512 1906 1481 2018"> <thead> <tr> <th data-bbox="512 1906 1026 1946">pH Display</th> <th data-bbox="1026 1906 1481 1946">Temperature Display</th> </tr> </thead> <tbody> <tr> <td data-bbox="512 1946 1026 1986">pH</td> <td data-bbox="1026 1946 1481 1986">Less than 0.0°C: $E \square 24$</td> </tr> <tr> <td data-bbox="512 1986 1026 2018">pH</td> <td data-bbox="1026 1986 1481 2018">Exceeding 110.0°C: $E \square 23$</td> </tr> </tbody> </table> | pH Display | Temperature Display | Less than pH 0.00: 0.00 | $\square F \square \square$ is flashing. | Exceeding pH 14.00: 14.00 | $\square F \square \square$ is flashing. | pH Display | Temperature Display | Less than pH 0.00: 0.00 is flashing. | Temperature | Exceeding pH 14.00: 14.00 is flashing. | Temperature | pH Display | Temperature Display | pH | Less than 0.0°C: $E \square 24$ | pH | Exceeding 110.0°C: $E \square 23$ |
| pH Display | Temperature Display | | | | | | | | | | | | | | | | | | |
| Less than pH 0.00: 0.00 | $\square F \square \square$ is flashing. | | | | | | | | | | | | | | | | | | |
| Exceeding pH 14.00: 14.00 | $\square F \square \square$ is flashing. | | | | | | | | | | | | | | | | | | |
| pH Display | Temperature Display | | | | | | | | | | | | | | | | | | |
| Less than pH 0.00: 0.00 is flashing. | Temperature | | | | | | | | | | | | | | | | | | |
| Exceeding pH 14.00: 14.00 is flashing. | Temperature | | | | | | | | | | | | | | | | | | |
| pH Display | Temperature Display | | | | | | | | | | | | | | | | | | |
| pH | Less than 0.0°C: $E \square 24$ | | | | | | | | | | | | | | | | | | |
| pH | Exceeding 110.0°C: $E \square 23$ | | | | | | | | | | | | | | | | | | |
| Power failure countermeasure | <p>The setting data is backed up in the non-volatile IC memory.</p> | | | | | | | | | | | | | | | | | | |
| Self-diagnosis | <p>The CPU is monitored by a watchdog timer, and if an abnormal status occurs, the WIL-102-PH is switched to warm-up status.</p> | | | | | | | | | | | | | | | | | | |

| | | | |
|--------------------|---|--|--|
| Warm-up indication | For approx. 4 seconds after the power is switched ON, the input characters are indicated on the pH Display and Temperature Display. Depending on the input specifications, Temperature Display indicates differently as follows. | | |
| | Pt spec | | |
| | pH Display | Temperature Display | Item selected in [Electrode RTD (p.28)] |
| | pH□□ | Unlit | nonE: No temperature compensation |
| | | PT 10 | PT 10: Pt1000 |
| | | PT 02 PT 03 | PT 10: Pt100 |
| | | | PT 02 : 2-wire type PT 03 : 3-wire type |
| Cu spec | | | |
| pH Display | Temperature Display | Item selected in [Electrode RTD (p.28)] | |
| pH□□ | Unlit | nonE: No temperature compensation | |
| | CU50 | CU50: Cu500 | |

| | |
|-------------------------|---|
| Display sleep function | 'pH', 'Temperature' or 'No indication' – which is indicated in pH/Temperature Display Mode, or Cleansing Output Mode – can be selected in [Display selection (p.32)]. If 'pH' or 'Temperature' is selected, and if indication time is set, the display (no operation status) becomes unlit after the indication time has passed. By pressing any key, the display re-lights. If the indication time is set to 0, the display remains lit, and this function does not work. |
| Auto-light function | Automatically measures and controls brightness of the pH Display, Temperature Display and action indicators. |
| Cable length correction | If PT 02 (2-wire type) is selected in [Pt100 input wire type (p.28)], and if sensor cable is too long, temperature measurement error will occur due to cable resistance. This can be corrected by setting the 'cable length correction value' and 'cable cross-section area'. |
| Zero indication | Indicates potential difference when pH 7 is calibrated. However, if Manual calibration is performed, zero indication value calculated at previous automatic calculation will not be updated. If calibration is not successfully completed, zero indication will show the value before calibration. |
| Slope indication | From the voltage equivalent to the calibrated pH, electromotive force for the change of pH 1 will be indicated. If calibration is not successfully completed, slope indication will show the value before calibration. |

| Error code | Error codes below flash on the Temperature Display. | | | | |
|------------|---|------------|------------------------------|--|-------------------------------|
| | Error Code | Error Type | Error Contents | Description | Occurrence |
| | E ₁₁ | Error | Response Speed Error | When calibrating, the response of the pH Combined Electrode Sensor is slow. When the difference between the input and each of the 1st and 2nd solutions are within pH ± 1.50 , and input fluctuation is over pH ± 0.05 (in 10 seconds of assessment cycles) for 5 minutes, this is assumed to be an error. However, if input fluctuation is less than or equal to pH ± 0.05 , this is assumed to be within the normal range. | When calibrating |
| | E ₁₂ | Error | Electrode Sensitivity Error | When calibrating, sensitivity of the pH Combined Electrode Sensor has deteriorated. The difference between 1st and 2nd standard solution value after calibration is less than or equal to pH 2.00. | |
| | E ₁₃ | Error | Asymmetry Potential Error | When calibrating pH 7, the difference in electromotive force between the sensor-measured value and standard value exceeds the equivalent of pH ± 1.50 . | |
| | E ₁₄ | Error | Standard Solution Error | The specified standard solution has not been used. When pH ± 1.50 is exceeded for the 1st and 2nd solutions. | |
| | E ₁₅ | Error | Solution temperature Error | When temperature is 55°C or more at pH 10 solution. | |
| | E ₂₁ | Fail | Temp. Sensor Burnout | Temperature sensor lead wire is burnt out. | When measuring or calibrating |
| | E ₂₂ | Fail | Temp. Sensor Short-circuited | Temperature sensor lead wire is short-circuited. | |
| | E ₂₃ | Error | Outside Temp. Compen.Range | Measured temperature has exceeded 110.0°C. | |
| | E ₂₄ | Error | Outside Temp. Compen.Range | Measured temperature is less than 0.0°C. | |

(Abbreviations: Temp.: Temperature, Compen.: Compensation)

Other

| | |
|-----------------------------|---|
| Power consumption | Approx. 8 VA |
| Ambient temperature | 0 to 50°C |
| Ambient humidity | 35 to 85 %RH (non-condensing) |
| Weight | Approx. 200 g (including the socket) |
| Accessories included | Instruction manual: 1 copy Unit label: 1 sheet |
| Accessories sold separately | Socket: ASK-001-1 (Finger-safe, terminal screw fall prevention) |
| Environmental specification | RoHS directive compliant |

12.2 Optional Specifications

A□□ Output (Option Code: EVT or TA)

| | | |
|---|---|--|
| A□□ output | <p>If the measured value exceeds the A□□ value, the A□□ output will be activated for each A□□ type.</p> <p>Regardless of options being ordered, A□□ output status can be read by reading Status flag 2 (A11, A12, A21, A22 output flag bit) in Serial communication.</p> <p>If <i>none</i> (No temperature compensation) is selected in [Electrode RTD (p.28)], Temperature input low limit and Temperature input high limit actions will not work.</p> <p>A□□ output status, when input errors occur, differs depending on the selections in [A□□ output when input errors occur (p.27)] as follows:</p> <ul style="list-style-type: none"> • If <i>OFF</i> (Disabled) is selected, the A□□ output and A□□ output status will be turned OFF if input errors occur. • If <i>ON</i> (Enabled) is selected, the A□□ output and A□□ output status will be maintained if input errors occur. <p>If Transmission output 1 (TA option) is ordered, only A1 output can be added.</p> | |
| Setting range | <p>pH input: pH 0.00 to 14.00 Temperature input: 0.0 to 100.0°C (The placement of the decimal point does not follow the selection. It is fixed.)</p> | |
| Action | ON/OFF action | |
| A□□ ON side A□□ OFF side | <p>pH input: pH 0.01 to 4.00 Temperature input: 0.1 to 10.0°C (The placement of the decimal point does not follow the selection. It is fixed.)</p> | |
| A□□ type | <p>One type can be selected from the following with the keypad.</p> <p>If 'No temperature compensation' is selected in [Electrode RTD (p.28)], Temperature input low limit and Temperature input high limit actions will not work.</p> <ul style="list-style-type: none"> • No action • pH input low limit action • pH input high limit action • Temperature input low limit action • Temperature input high limit action • Error output: The A□□ output will be turned ON when the error type is 'Error'. (Table 9.1.3-1, p.41) • Fail output: The A□□ output will be turned ON when the error type is 'Fail'. (Table 9.1.3-1, p.41) • Cleansing output • pH fluctuation alarm output • pH input High/Low limits independent action • Temperature input High/Low limits independent action | |
| Output | Relay contact, 1a | |
| | Control capacity | <p>3 A 250 V AC (resistive load) 1 A 250 V AC (inductive load, $\cos\phi=0.4$)</p> |
| | Electrical life | 100,000 cycles |
| A□□ ON delay time | 0 to 9999 seconds | |
| A□□ OFF delay time | 0 to 9999 seconds | |
| A1, A2 output allocation | <p>A11 type, A12 type, A21 type and/or A22 type are allocated to A1 (or A2) output. Output is OR output. However, if Cleansing output is selected in any one of [A11, A12, A21, A22 type], the Cleansing output will be given priority.</p> | |
| Output ON time/ OFF time when A1/A2 output ON | <p>If Output ON time and OFF time are set, A1 (or A2) output can be turned ON/OFF in a configured cycle when A1 (or A2) output is ON.</p> | |

| | |
|-----------------------------|--|
| pH input error alarm | <p>Detects actuator trouble.</p> <p>Even if pH input error alarm time has elapsed – if the change in pH input is smaller than the pH input error alarm band – the instrument assumes that actuator trouble has occurred, and sets Status flag 2 (A1, A2 pH input error alarm output flag bit).</p> <p>In Serial communication, status can be read by reading Status flag 2 (A1, A2 pH input error alarm output flag bit).</p> <p>When pH is calibrated, this alarm is disabled.</p> <p>If PH_L (pH input low limit action) or PH_H (pH input high limit action) is selected in [A11, A12, A21, A22 type (pp.21, 22)], this alarm is enabled.</p> |
| pH fluctuation alarm output | <p>Detects pH fluctuation errors.</p> <p>Even if pH fluctuation alarm time has elapsed, – if the change in pH input fluctuation is smaller than the pH fluctuation alarm band – the instrument assumes that a pH fluctuation error has occurred, and sets Status flag 2 (A11, A12, A21, A22 output flag bit).</p> <p>Outputs when $EPHA$ (pH fluctuation alarm output) is selected in [A11, A12, A21, A22 type (pp.21, 22)].</p> <p>This alarm will be disabled if pH fluctuation alarm time is set to 0 (zero) hours, or if pH fluctuation alarm band is set to pH 0.00.</p> |

Transmission Output 1 (Option Code: TA)

| | | | | | | | |
|---|--|------------|-------|---------|--|-----------------|--|
| Transmission output 1 | <p>Converting pH or temperature to analog signal every input sampling period, and outputs the value in current.</p> <p>If $NOCT$ (No temperature compensation) is selected in [Electrode RTD (p.28)], and if $TEMP$ (Temperature transmission) is selected in [Transmission output 1 type (p.30)], the value set in [Reference temperature (p.28)] will be output.</p> <p>If Transmission output 1 high limit and low limit are set to the same value, Transmission output 1 will be fixed at 4 mA DC. (The placement of the decimal point does not follow the selection. It is fixed.)</p> <table border="1"> <tr> <td>Resolution</td> <td>12000</td> </tr> <tr> <td>Current</td> <td>4 to 20 mA DC (Load resistance: Max 550 Ω)</td> </tr> <tr> <td>Output accuracy</td> <td>Within $\pm 0.3\%$ of Transmission output 1 Span</td> </tr> </table> | Resolution | 12000 | Current | 4 to 20 mA DC (Load resistance: Max 550 Ω) | Output accuracy | Within $\pm 0.3\%$ of Transmission output 1 Span |
| Resolution | 12000 | | | | | | |
| Current | 4 to 20 mA DC (Load resistance: Max 550 Ω) | | | | | | |
| Output accuracy | Within $\pm 0.3\%$ of Transmission output 1 Span | | | | | | |
| Transmission output 1 adjustment | Fine adjustment of Transmission output 1 can be performed via Transmission output 1 Zero adjustment and Span adjustment. | | | | | | |
| Transmission output 1 status when calibrating | <p>Transmission output 1 status can be selected when calibrating pH.</p> <p>Last value HOLD: Retains the last value before pH calibration, and outputs it.</p> <p>Set value HOLD: Outputs the value set in [Transmission output 1 value HOLD when calibrating].</p> <p>Measured value: Outputs the measured value when calibrating pH.</p> | | | | | | |

Transmission Output 2 (Option Code: TA2)

| | | | | | | | |
|---|--|------------|-------|---------|--|-----------------|--|
| Transmission output 2 | <p>Converting pH or temperature to analog signal every input sampling period, and outputs the value in current.</p> <p>If $NOCT$ (No temperature compensation) is selected in [Electrode RTD (p.28)], and if $TEMP$ (Temperature transmission) is selected in [Transmission output 2 type (p.30)], the value set in [Reference temperature (p.28)] will be output.</p> <p>If Transmission output 2 high limit and low limit are set to the same value, Transmission output 2 will be fixed at 4 mA DC. (The placement of the decimal point does not follow the selection. It is fixed.)</p> <table border="1"> <tr> <td>Resolution</td> <td>12000</td> </tr> <tr> <td>Current</td> <td>4 to 20 mA DC (Load resistance: Max 550 Ω)</td> </tr> <tr> <td>Output accuracy</td> <td>Within $\pm 0.3\%$ of Transmission output 2 Span</td> </tr> </table> | Resolution | 12000 | Current | 4 to 20 mA DC (Load resistance: Max 550 Ω) | Output accuracy | Within $\pm 0.3\%$ of Transmission output 2 Span |
| Resolution | 12000 | | | | | | |
| Current | 4 to 20 mA DC (Load resistance: Max 550 Ω) | | | | | | |
| Output accuracy | Within $\pm 0.3\%$ of Transmission output 2 Span | | | | | | |
| Transmission output 2 adjustment | Fine adjustment of Transmission output 2 can be performed via Transmission output 2 Zero adjustment and Span adjustment. | | | | | | |
| Transmission output 2 status when calibrating | <p>Transmission output 2 status can be selected when calibrating pH.</p> <p>Last value HOLD: Retains the last value before pH calibration, and outputs it.</p> <p>Set value HOLD: Outputs the value set in [Transmission output 2 value HOLD when calibrating].</p> <p>Measured value: Outputs the measured value when calibrating pH.</p> | | | | | | |

13. Troubleshooting

If any malfunction occurs, refer to the following items after checking that power is being supplied to the WIL-102-PH.

13.1 Indication

| Problem | Possible Cause | Solution |
|--|--|--|
| The pH/Temperature Display is unlit. | None (No Indication) is selected in [Display selection (p.32)]. | Select ALL (pH/Temperature). |
| | The time set in [Indication time (p.32)] has passed. | If any key is pressed while displays are unlit, it will re-light. Set the indication time to a suitable time-frame. |
| The pH/Temperature Display is dark. | Auto-light (Enabled) is selected in [Auto-light function (p.31)]. | Select Auto-light (Disabled). |
| Indication of the pH/Temperature Display is unstable or irregular. | pH calibration and temperature calibration may not have finished. | Perform pH calibration and temperature calibration. |
| | Electrode RTD selection might not be correct. | Select a correct electrode RTD. |
| | Specification of the pH Combined Electrode Sensor may not be suitable. | Replace the sensor with a suitable one. |
| | There may be equipment that interferes with or makes noise near the WIL-102-PH. | Keep WIL-102-PH clear of any potentially disruptive equipment. Try [Grounding of shield wire terminal (E) (P.78)]. |
| Temperature Display is unlit. | Temp Display (Unlit) is selected in [Temperature Display when no temperature compensation (p.32)]. | Select Temp Display (Reference temperature). |
| [E 11] is flashing on the Temperature Display. | This shows that the response of the pH Combined Electrode Sensor is slow when calibrating. | Rinse the pH Combined Electrode Sensor. If [E 11] is still flashing, check if the standard solution and pH Combined Electrode Sensor are normal. If they are not normal, replace the solution or the sensor. |
| [E 12] is flashing on the Temperature Display. | This shows that pH electrode sensitivity has deteriorated when calibrating. | Rinse the pH Combined Electrode Sensor, and refill the internal solution. If [E 12] is still flashing, replace the sensor. |
| [E 13] is flashing on the Temperature Display. | When calibrating, electromotive force (asymmetry potential) of pH 7 is large. | Rinse the pH Combined Electrode Sensor, and refill the internal solution. If [E 13] is still flashing, replace the sensor. |
| [E 14] is flashing on the Temperature Display. | When calibrating, the specified standard solution is not used. | Rinse the pH combined electrode sensor, and refill the internal solution. If [E 14] is still flashing, use the specified standard solution. |
| [E 15] is flashing on the Temperature Display. | When calibrating, temperature of pH 10 is 55°C or higher. | Check the liquid temperature of pH 10. |

| Problem | Possible Cause | Solution |
|--|---|--|
| [E021] is flashing on the Temperature Display. | This occurs when the temperature sensor lead wire is burnt out. | Replace the pH Combined Electrode Sensor. |
| [E022] is flashing on the Temperature Display. | This occurs when the temperature sensor lead wire is short-circuited. | Replace the pH Combined Electrode Sensor. |
| [E023] is flashing on the Temperature Display. | This occurs when measured temperature value exceeds 110.0°C. | Check the environment of measurement location. |
| [E024] is flashing on the Temperature Display. | This occurs when measured temperature value is less than 0.0°C. | Check the environment of measurement location. |
| [Err1] is indicating on the pH Display. | Internal memory is defective. | Contact our agency or us. |


• Grounding of shield wire terminal (E)

If the indication fluctuates due to noise, ground the shield wire terminal (E).

However, depending on the installation environment, the symptom may not be improved.

In this case, disconnect the grounding of the shield wire terminal (E) and return it to the original state.

(Depending on the type of sensor, the cable for the shield wire terminal (E) may not be available.)

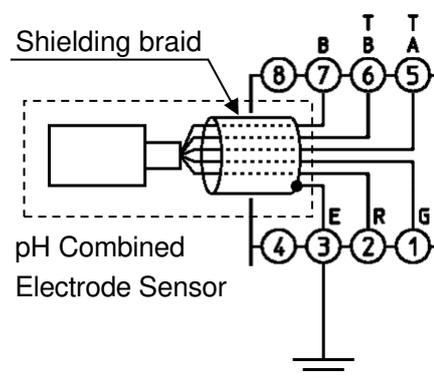

13.2 Key Operation

| Problem | Possible Cause | Solution |
|---|--|--|
| <ul style="list-style-type: none"> None of the set values can be changed. The values do not change by the and keys. | $Loc 1$ (Lock 1) is selected in [Set value lock (p.29)]. | Select (Unlock). |
| <ul style="list-style-type: none"> Only $A□□$ value can be set. Other settings are not possible. The values do not change by the and keys. | $Loc 2$ (Lock 2) is selected in [Set value lock (p.29)]. | Select (Unlock). |
| Unable to enter Manual cleansing mode. | $cLEU$ (Cleansing output) is not selected in any one of [A11, A12, A21 or A22 type (pp. 21, 22)]. | Select $cLEU$ (Cleansing output) in any one of [A11, A12, A21 or A22 type (pp. 21, 22)]. |
| | Cleansing action is performing using the 'Cleansing time' and 'Restore time after cleansing' settings. | Execute Manual cleansing after Cleansing action is completed. |
| Unable to enter a calibration mode (pH calibration mode or Temperature calibration mode). | $Loc 1$ (Lock 1), $Loc 2$ (Lock 2) or $Loc 3$ (Lock 3) is selected in [Set value lock (p.29)]. | Select (Unlock). |
| | $cLEU$ (Cleansing output) has been selected in any one of [A11, A12, A21, A22 type (pp. 21, 22)], and cleansing action is performing using the 'Cleansing Time' and 'Restore Time after Cleansing' settings. | Perform calibration after cleansing action is completed. |

13.3 Communication

Check that power is being supplied to the master and slave that customers use.

If communication failure still occurs, check the following.

| Problem | Possible Cause | Solution |
|--|---|---|
| Communication failure | Communication cable is not securely connected, or is disconnected/defective. | Check the communication cable and connector. |
| | Incorrect wiring of the communication cable and/or connector | Check the communication cable and connector. |
| | Imperfect contact between the communication cable and the connector, or between the communication connector and instrument port | Check the communication cable and connector. |
| | Communication speed of the slave does not match that of the master. | Check the communication speed of the slave and master. |
| | The data bit, parity and stop bit of the master do not correspond to those of the slave. | Check the data bit, parity and stop bit of the master and the slave. |
| | The instrument number (address) of the slave does not correspond to that of the command. | Check the instrument number (address) of the slave and command. |
| | The instrument numbers (addresses) are duplicated in multiple slaves. | Check the instrument numbers (addresses) of the slave. |
| | Make sure that the program is appropriate for the transmission timing. | Check the program. |
| Although communication is occurring, the response is negative acknowledgement. | A non-existent command code has been sent. | Check the command code. |
| | The setting command data exceeds the setting range of the slave. | Check the setting range of the slave. |
| | The WIL-102-PH cannot be set while calibration is being performed using the Automatic electrode quality evaluation function. | Check the slave status. |
| | The WIL-102-PH is in front keypad operation setting mode. | Return the instrument to pH/Temperature Display Mode, or Cleansing Output Mode. |

For all other malfunctions, please contact our main office or dealers.

14. Character Tables

The following shows our character tables. Use data column for your reference.

Setting Groups

| Character | Setting Group |
|-----------|-----------------------------|
| F.n.c.1 | pH Input Group |
| F.n.c.2 | Temperature Input Group |
| a.f.f.r | Basic Function Group |
| z.r.h.P | Zero/Slope Indication Group |

Temperature Calibration Mode

| Character | Setting Item, Setting Range | Factory Default | Data |
|-----------|--------------------------------|-----------------|------|
| 40.00 (*) | Temperature calibration value | 0.0°C | |
| 00.00 | Setting range: -10.0 to 10.0°C | | |

(*) 40.00 and temperature are displayed alternately.

pH Calibration Mode (for pH manual calibration)

| Character | Setting Item, Setting Range | Factory Default | Data |
|-----------|------------------------------|-----------------|------|
| 8.10 (*) | pH calibration value | 0.00 | |
| 00.00 | Setting range: -7.00 to 7.00 | | |

(*) 8.10 and pH are displayed alternately.

Transmission Output 1 Adjustment Mode

| Character | Setting Item, Setting Range | Factory Default | Data |
|-----------|---|-----------------|------|
| AJ3.1 | Transmission output 1 Zero adjustment value | 0.00% | |
| 00.00 | Setting range: ±5.00% of Transmission output 1 Span | | |
| AJ4.1 | Transmission output 1 Span adjustment value | 0.00% | |
| 00.00 | Setting range: ±5.00% of Transmission output 1 Span | | |

Transmission Output 2 Adjustment Mode

| Character | Setting Item, Setting Range | Factory Default | Data |
|-----------|---|-----------------|------|
| AJ3.2 | Transmission output 2 Zero adjustment value | 0.00% | |
| 00.00 | Setting range: ±5.00% of Transmission output 2 Span | | |
| AJ4.2 | Transmission output 2 Span adjustment value | 0.00% | |
| 00.00 | Setting range: ±5.00% of Transmission output 2 Span | | |

pH Input Group

| Character | Setting Item, Setting Range | Factory Default | Data |
|-----------------------------|---|---|------|
| <i>TYPE</i> <i>J1 4</i> | pH 7 calibration standard <i>J1 4</i> : JIS (Japanese Industrial Standards) <i>U4</i> : US standard | JIS | |
| <i>4EPH</i> <i>PH4</i> | 2nd solution <i>PH2</i> : pH 2 <i>PH4</i> : pH 4 <i>PH9</i> : pH 9 <i>PH 10</i> : pH 10 | pH 4 | |
| <i>dp 1</i> <i>000</i> | Decimal point place <i>000</i> : No decimal point <i>00</i> : 1 digit after decimal point <i>000</i> : 2 digits after decimal point | 2 digits after decimal point | |
| <i>A11F</i> <i>----</i> | A11 type <i>----</i> : No action <i>PH_L</i> : pH input low limit action <i>PH_H</i> : pH input high limit action <i>TEMP_L</i> : Temperature input low limit action <i>TEMP_H</i> : Temperature input high limit action <i>ERR</i> : Error output <i>FAIL</i> : Fail output <i>CLSD</i> : Cleansing output <i>EPHA</i> : pH fluctuation alarm output <i>PHHL</i> : pH input High/Low limits independent action <i>TEMP_HL</i> : Temperature input High/Low limits independent action | No action | |
| <i>A12F</i> <i>----</i> | A12 type Selection item: Same as those of [A11 type] | No action | |
| <i>A21F</i> <i>----</i> | A21 type Selection item: Same as those of [A11 type] | No action | |
| <i>A22F</i> <i>----</i> | A22 type Selection item: Same as those of [A11 type] | No action | |
| <i>A11</i> <i>000</i> | A11 value Setting range: pH input low limit, high limit actions: pH 0.00 to 14.00 (*) Temperature input low limit, high limit actions: 0.0 to 100.0°C (*) | pH input: pH 0.00, Temperature input: 0.0°C | |
| <i>A12</i> <i>000</i> | A12 value Setting range: Same as those of [A11 value] | pH input: pH 0.00, Temperature input: 0.0°C | |
| <i>A21</i> <i>000</i> | A21 value Setting range: Same as those of [A11 value] | pH input: pH 0.00, Temperature input: 0.0°C | |
| <i>A22</i> <i>000</i> | A22 value Setting range: Same as those of [A11 value] | pH input: pH 0.00, Temperature input: 0.0°C | |
| <i>A11d</i> <i>4dl F</i> | A11 hysteresis type <i>4dl F</i> : Medium Value <i>4dl F</i> : Reference Value | Reference Value | |
| <i>A11U</i> <i>0.10</i> | A11 ON side Setting range: pH input: pH 0.00 to 4.00 (*) Temperature input: 0.0 to 10.0°C (*) | pH input: pH 0.10, Temperature input: 1.0°C | |
| <i>A11L</i> <i>0.10</i> | A11 OFF side Setting range: pH input: pH 0.00 to 4.00 (*) Temperature input: 0.0 to 10.0°C (*) | pH input: pH 0.10, Temperature input: 1.0°C | |

(*) The placement of the decimal point does not follow the selection. It is fixed.

| Character | Setting Item, Setting Range | Factory Default | Data |
|--------------|---|---|------|
| A12d 4d1F | A12 hysteresis type Selection item: Same as those of [A11 hysteresis type] (p.81) | Reference Value | |
| A12U 0.10 | A12 ON side Setting range: Same as those of [A11 ON side] (p.81) | pH input: pH 0.10, Temperature input: 1.0°C | |
| A12L 0.10 | A12 OFF side Setting range: Same as those of [A11 OFF side] (p.81) | pH input: pH 0.10, Temperature input: 1.0°C | |
| A21d 4d1F | A21 hysteresis type Selection item: Same as those of [A11 hysteresis type] (p.81) | Reference Value | |
| A21U 0.10 | A21 ON side Setting range: Same as those of [A11 ON side] (p.81) | pH input: pH 0.10, Temperature input: 1.0°C | |
| A21L 0.10 | A21 OFF side Setting range: Same as those of [A11 OFF side] (p.81) | pH input: pH 0.10, Temperature input: 1.0°C | |
| A22d 4d1F | A22 hysteresis type Selection item: Same as those of [A11 hysteresis type] (p.81) | Reference Value | |
| A22U 0.10 | A22 ON side Setting range: Same as those of [A11 ON side] (p.81) | pH input: pH 0.10, Temperature input: 1.0°C | |
| A22L 0.10 | A22 OFF side Setting range: Same as those of [A11 OFF side] (p.81) | pH input: pH 0.10, Temperature input: 1.0°C | |
| A11a 0000 | A11 ON delay time Setting range: 0 to 9999 seconds | 0 seconds | |
| A12a 0000 | A12 ON delay time Setting range: 0 to 9999 seconds | 0 seconds | |
| A21a 0000 | A21 ON delay time Setting range: 0 to 9999 seconds | 0 seconds | |
| A22a 0000 | A22 ON delay time Setting range: 0 to 9999 seconds | 0 seconds | |
| A11c 0000 | A11 OFF delay time Setting range: 0 to 9999 seconds | 0 seconds | |
| A12c 0000 | A12 OFF delay time Setting range: 0 to 9999 seconds | 0 seconds | |
| A21c 0000 | A21 OFF delay time Setting range: 0 to 9999 seconds | 0 seconds | |
| A22c 0000 | A22 OFF delay time Setting range: 0 to 9999 seconds | 0 seconds | |
| A11f 0000 | A11 pH fluctuation alarm time Setting range: 0 to 72 hours | 0 hours | |
| A12f 0000 | A12 pH fluctuation alarm time Setting range: 0 to 72 hours | 0 hours | |
| A21f 0000 | A21 pH fluctuation alarm time Setting range: 0 to 72 hours | 0 hours | |
| A22f 0000 | A22 pH fluctuation alarm time Setting range: 0 to 72 hours | 0 hours | |
| A114 0000 | A11 pH fluctuation alarm band Setting range: pH 0.00 to 14.00 | pH 0.00 | |
| A124 0000 | A12 pH fluctuation alarm band Setting range: pH 0.00 to 14.00 | pH 0.00 | |
| A214 0000 | A21 pH fluctuation alarm band Setting range: pH 0.00 to 14.00 | pH 0.00 | |

| Character | Setting Item, Setting Range | Factory Default | Data |
|---------------|--|---|------|
| A224 □000 | A22 pH fluctuation alarm band Setting range: pH 0.00 to 14.00 | pH 0.00 | |
| A11n □000 | A11 High/Low limits independent lower side band Setting range: pH input: pH 0.00 to 14.00 (*) Temperature input: 0.0 to 100.0°C (*) | pH input: pH 0.00 Temperature input: 0.0°C | |
| A12n □000 | A12 High/Low limits independent lower side band Setting range: Same as those of [A11 High/Low limits independent lower side band] | pH input: pH 0.00 Temperature input: 0.0°C | |
| A21n □000 | A21 High/Low limits independent lower side band Setting range: Same as those of [A11 High/Low limits independent lower side band] | pH input: pH 0.00 Temperature input: 0.0°C | |
| A22n □000 | A22 High/Low limits independent lower side band Setting range: Same as those of [A11 High/Low limits independent lower side band] | pH input: pH 0.00 Temperature input: 0.0°C | |
| A11P □000 | A11 High/Low limits independent upper side band Setting range: pH input: pH 0.00 to 14.00 (*) Temperature input: 0.0 to 100.0°C (*) | pH input: pH 0.00 Temperature input: 0.0°C | |
| A12P □000 | A12 High/Low limits independent upper side band Setting range: Same as those of [A11 High/Low limits independent upper side band] | pH input: pH 0.00 Temperature input: 0.0°C | |
| A21P □000 | A21 High/Low limits independent upper side band Setting range: Same as those of [A11 High/Low limits independent upper side band] | pH input: pH 0.00 Temperature input: 0.0°C | |
| A22P □000 | A22 High/Low limits independent upper side band Setting range: Same as those of [A11 High/Low limits independent upper side band] | pH input: pH 0.00 Temperature input: 0.0°C | |
| A11H □0.10 | A11 hysteresis Setting range: pH input: pH 0.01 to 4.00 (*) Temperature input: 0.1 to 10.0°C (*) | pH input: pH 0.10 Temperature input: 1.0°C | |
| A12H □0.10 | A12 hysteresis Setting range: Same as those of [A11 hysteresis] | pH input: pH 0.10 Temperature input: 1.0°C | |
| A21H □0.10 | A21 hysteresis Setting range: Same as those of [A11 hysteresis] | pH input: pH 0.10 Temperature input: 1.0°C | |
| A22H □0.10 | A22 hysteresis Setting range: Same as those of [A11 hysteresis] | pH input: pH 0.10 Temperature input: 1.0°C | |
| 1Err oFF□ | A□□ output when input errors occur Selection item: on□□ : Enabled oFF□ : Disabled | Disabled | |
| FILT □□00 | pH input filter time constant Setting range: 0.0 to 60.0 seconds | 0.0 seconds | |
| P4o□ □000 | pH input sensor correction Setting range: pH -1.40 to 1.40 (*) | 0.00 | |
| dFcT □20 | pH inputs for moving average Setting range: 1 to 120 | 20 | |

(*) The placement of the decimal point does not follow the selection. It is fixed.

Temperature Input Group

| Character | Setting Item, Setting Range | Factory Default | Data |
|-----------------------------|--|-----------------------------------|------|
| <i>4En4</i> <i>PF 10</i> | Electrode RTD Pt spec <i>nonE</i> : No temperature compensation <i>PF 10</i> : Pt1000 <i>PF 10</i> : Pt100 Cu spec <i>nonE</i> : No temperature compensation <i>cU50</i> : Cu500 | Pt spec: Pt1000 Cu spec: Cu500 | |
| <i>4Fnd</i> <i>0250</i> | Reference temperature Setting range: 5.0 to 95.0°C (*) | 25.0°C | |
| <i>dP20</i> <i>0000</i> | Decimal point place <i>0000</i> : No decimal point <i>0000</i> : 1 digit after decimal point | 1 digit after decimal point | |
| <i>cOnE</i> <i>PF 03</i> | Pt100 input wire type <i>PF 02</i> : 2-wire type <i>PF 03</i> : 3-wire type | 3-wire type | |
| <i>cAbL</i> <i>0000</i> | Cable length correction Setting range: 0.0 to 100.0 m | 0.0 m | |
| <i>c4Ec</i> <i>0030</i> | Cable cross-section area Setting range: 0.10 to 2.00 mm ² | 0.30 mm ² | |
| <i>dFcf</i> <i>0020</i> | Temperature inputs for moving average Setting range: 1 to 120 | 20 | |

(*) The placement of the decimal point does not follow the selection. It is fixed.

Basic Function Group

| Character | Setting Item, Setting Range | Factory Default | Data |
|----------------------------|--|-----------------|------|
| <i>Locb</i> <i>0000</i> | Set value lock <i>0000</i> : Unlock <i>Loc 1</i> : Lock 1 <i>Loc 2</i> : Lock 2 <i>Loc 3</i> : Lock 3 | Unlock | |
| <i>cñ4L</i> <i>nonL</i> | Communication protocol <i>nonL</i> : Shinko protocol <i>ñodA</i> : MODBUS ASCII mode <i>ñodr</i> : MODBUS RTU mode | Shinko protocol | |
| <i>cñno</i> <i>0000</i> | Instrument number Setting range: 0 to 95 | 0 | |
| <i>cñ4P</i> <i>0096</i> | Communication speed <i>0096</i> : 9600 bps <i>0192</i> : 19200 bps <i>0384</i> : 38400 bps | 9600 bps | |
| <i>cñFF</i> <i>7EBn</i> | Data bit/Parity <i>8non</i> : 8 bits/No parity <i>7non</i> : 7 bits/No parity <i>8EBn</i> : 8 bits/Even <i>7EBn</i> : 7 bits/Even <i>8odd</i> : 8 bits/Odd <i>7odd</i> : 7 bits/Odd | 7 bits/Even | |

| Character | Setting Item, Setting Range | Factory Default | Data | | | | | | | | | | | | | | | |
|-----------------------------|--|---|------------|---------------------|--------------|----|-------------|--------------|----|---------------|-------------|---------------|-------------|-------------|---------------|---------------|----------------|--|
| <i>cā4f</i> □□□1 | Stop bit □□□1 : 1 bit □□□2 : 2 bits | 1 bit | | | | | | | | | | | | | | | | |
| <i>Frō1</i> <i>PH</i> □□ | Transmission output 1 type <i>PH</i> □□ : pH transmission <i>TEāP</i> : Temperature transmission | pH transmission | | | | | | | | | | | | | | | | |
| <i>FrH1</i> 1400 | Transmission output 1 high limit pH transmission: Transmission output 1 low limit to pH 14.00 (*) Temperature transmission: Transmission output 1 low limit to 100.0°C(*) | pH 14.00 | | | | | | | | | | | | | | | | |
| <i>FrL1</i> □000 | Transmission output 1 low limit pH transmission: pH 0.00 to Transmission output 1 high limit (*) Temperature transmission: 0.0°C to Transmission output 1 high limit (*) | pH 0.00 | | | | | | | | | | | | | | | | |
| <i>Frō2</i> <i>TEāP</i> | Transmission output 2 type Selection item: Same as those of [Transmission output 1 type] | Temperature transmission | | | | | | | | | | | | | | | | |
| <i>FrH2</i> 1000 | Transmission output 2 high limit Setting range: Same as those of [Transmission output 1 high limit] | 100.0°C | | | | | | | | | | | | | | | | |
| <i>FrL2</i> □000 | Transmission output 2 low limit Setting range: Same as those of [Transmission output 1 low limit] | 0.0°C | | | | | | | | | | | | | | | | |
| <i>Frō1</i> <i>bEFH</i> | Transmission output 1 status when calibrating <i>bEFH</i> : Last value HOLD <i>4EFH</i> : Set value HOLD <i>PH</i> □ : Measured value | Last value HOLD | | | | | | | | | | | | | | | | |
| <i>Fr41</i> □000 | Transmission output 1 value HOLD when calibrating pH transmission : pH 0.00 to 14.00 (*) Temperature transmission : 0.0 to 100.0°C (*) | pH transmission: pH 0.00 Temperature transmission: 0.0°C | | | | | | | | | | | | | | | | |
| <i>Frō2</i> <i>bEFH</i> | Transmission output 2 status when calibrating Selection item: Same as those of [Transmission output 1 status when calibrating] | Last value HOLD | | | | | | | | | | | | | | | | |
| <i>Fr42</i> □000 | Transmission output 2 value HOLD when calibrating Setting range: Same as those of [Transmission output 1 value HOLD when calibrating] | pH transmission: pH 0.00 Temperature transmission: 0.0°C | | | | | | | | | | | | | | | | |
| <i>RJ4f</i> <i>RUFō</i> | pH calibration Auto/Manual <i>RUFō</i> : Automatic <i>āRāU</i> : Manual | Automatic | | | | | | | | | | | | | | | | |
| <i>L1ōf</i> - - - - | Auto-light function - - - - : Disabled <i>U4E□</i> : Enabled | Disabled | | | | | | | | | | | | | | | | |
| <i>d14P</i> <i>ALL</i> □ | Display selection <table border="1" data-bbox="395 1765 1252 1962"> <thead> <tr> <th></th> <th>pH Display</th> <th>Temperature Display</th> </tr> </thead> <tbody> <tr> <td><i>ALL</i>□</td> <td>pH</td> <td>Temperature</td> </tr> <tr> <td><i>PH</i>□□</td> <td>pH</td> <td>No indication</td> </tr> <tr> <td><i>TEāP</i></td> <td>No indication</td> <td>Temperature</td> </tr> <tr> <td><i>nonE</i></td> <td>No indication</td> <td>No indication</td> </tr> </tbody> </table> | | pH Display | Temperature Display | <i>ALL</i> □ | pH | Temperature | <i>PH</i> □□ | pH | No indication | <i>TEāP</i> | No indication | Temperature | <i>nonE</i> | No indication | No indication | pH/Temperature | |
| | pH Display | Temperature Display | | | | | | | | | | | | | | | | |
| <i>ALL</i> □ | pH | Temperature | | | | | | | | | | | | | | | | |
| <i>PH</i> □□ | pH | No indication | | | | | | | | | | | | | | | | |
| <i>TEāP</i> | No indication | Temperature | | | | | | | | | | | | | | | | |
| <i>nonE</i> | No indication | No indication | | | | | | | | | | | | | | | | |
| <i>FlāE</i> 0000 | Indication time 00.00 (Remains lit) 00.01 to 60.00 (Minutes.Seconds) | 00.00 | | | | | | | | | | | | | | | | |

(*) The placement of the decimal point does not follow the selection. It is fixed.

| Character | Setting Item, Setting Range | Factory Default | Data |
|--------------------------------|---|-----------------|------|
| <i>aFdP</i> <i>aFF</i> □ | Temperature Display when no temperature compensation <i>rTd</i> □ : Reference temperature <i>aFF</i> □ : Unlit | Unlit | |
| <i>R1oF</i> <i>R1</i> □ | A1 output allocation <i>R1</i> □ : A11 type <i>R12</i> □ : A12 type <i>R21</i> □ : A21 type <i>R22</i> □ : A22 type <i>R1A1</i> : A11, A12 types <i>R2A1</i> : A21, A22 types <i>R1A2</i> : A11, A21 types <i>R2A2</i> : A12, A22 types <i>ALL</i> □ : A11, A12, A21, A22 types | A11 type | |
| <i>R2oF</i> <i>R2</i> □ | A2 output allocation Selection item: Same as those of [A1 output allocation] | A21 type | |
| <i>oon1</i> □□□□ | Output ON time when A1 output ON Setting range: 0 to 9999 seconds | 0 seconds | |
| <i>oof1</i> □□□□ | Output OFF time when A1 output ON Setting range: 0 to 9999 seconds | 0 seconds | |
| <i>oon2</i> □□□□ | Output ON time when A2 output ON Setting range: 0 to 9999 seconds | 0 seconds | |
| <i>oof2</i> □□□□ | Output OFF time when A2 output ON Setting range: 0 to 9999 seconds | 0 seconds | |
| <i>R1P</i> □ □□□□ | A1 pH input error alarm A□□ type □□□□ : No action <i>R1</i> □ : A11 type <i>R12</i> □ : A12 type <i>R21</i> □ : A21 type <i>R22</i> □ : A22 type | No action | |
| <i>R2P</i> □ □□□□ | A2 pH input error alarm A□□ type Selection item: Same as [A1 pH input error alarm A□□ type]. | No action | |
| <i>R1P_a</i> □□□□ | A1 pH input error alarm band when A□□ output ON Setting range: pH 0.00 to 14.00 | pH 0.00 | |
| <i>R1oT</i> □□□□ | A1 pH input error alarm time when A□□ output ON Setting range: 0 to 9999 seconds or minutes (*) | 0 seconds | |
| <i>R1P_c</i> □□□□ | A1 pH input error alarm band when A□□ output OFF Setting range: pH 0.00 to 14.00 | pH 0.00 | |
| <i>R1oT</i> □□□□ | A1 pH input error alarm time when A□□ output OFF Setting range: 0 to 9999 seconds or minutes (*) | 0 seconds | |
| <i>R2P_a</i> □□□□ | A2 pH input error alarm band when A□□ output ON Setting range: pH 0.00 to 14.00 | pH 0.00 | |

(*) The time unit depends on the selection in [pH input error alarm time unit].

| Character | Setting Item, Setting Range | Factory Default | Data |
|--------------|---|---|------|
| A2oF □□□□ | A2 pH input error alarm time when A□□ output ON Setting range: 0 to 9999 seconds or minutes (*1) | 0 seconds | |
| A2Pc □□□□ | A2 pH input error alarm band when A□□ output OFF Setting range: pH 0.00 to 14.00 | pH 0.00 | |
| A2cF □□□□ | A2 pH input error alarm time when A□□ output OFF Setting range: 0 to 9999 seconds or minutes (*1) | 0 seconds | |
| n_4□ 4Ec□ | pH input error alarm time unit 4Ec□: Second(s) n/n□: Minute(s) | Second(s) | |
| ccnF □□□□ | Number of cleansing cycles Setting range: 0 to 10 (0: Continuous cleansing) | 0 (Continuous cleansing) | |
| cc4c □360 | Cleansing interval Setting range: 60 to 3000 minutes | 360 minutes | |
| cf1n □600 | Cleansing time Setting range: 1 to 1800 seconds | 600 seconds | |
| crEc □600 | Restore time after cleansing Setting range: 1 to 1800 seconds | 600 seconds | |
| cc41 bEFH | Transmission output 1 status when cleansing bEFH : Last value HOLD 4EFH : Set value HOLD PHH□ : Measured value | Last value HOLD | |
| ccE1 □□□□ | Transmission output 1 value HOLD when cleansing pH transmission : pH 0.00 to 14.00 (*2) Temperature transmission : 0.0 to 100.0°C (*2) | pH transmission: pH 0.00 Temperature transmission: 0.0°C | |
| cc42 bEFH | Transmission output 2 status when cleansing Selection item: Same as [Transmission output 1 status when cleansing] | Last value HOLD | |
| ccE2 □□□□ | Transmission output 2 value HOLD when cleansing Selection item: Same as [Transmission output 1 value HOLD when cleansing] | pH transmission: pH 0.00 Temperature transmission: 0.0°C | |

(*1) The time unit depends on the selection in [pH input error alarm time unit].

(*2) The placement of the decimal point does not follow the selection. It is fixed.

Zero/Slope Indication Group

| Character | Setting Item, Indication Range | Factory Default | Data |
|--------------|---|-----------------|------|
| ZEro □□□□ | Zero indication Indication range: Voltage equivalent to pH ±1.5 | 0.0 mV | |
| 4LoP □592 | Slope indication Indication range: Voltage equivalent to pH 0.00 to 14.00 | 59.2 mV | |

***** Inquiries *****

For any inquiries about this unit, please contact our agency or the vendor where you purchased the unit after checking the following.

[Example]

- Model ----- WIL-102-PH
- Serial number ----- No. 195F05000

In addition to the above, please let us know the details of the malfunction / discrepancy, and the operating conditions.

SHINKO TECHNOS CO., LTD.
OVERSEAS DIVISION

Head Office: 2-5-1, Senbahigashi, Minoo, Osaka, 562-0035, Japan

[URL] <https://shinko-technos.co.jp/e/>

[E-mail] overseas@shinko-technos.co.jp

Tel: +81-72-727-6100

Fax: +81-72-727-7006